
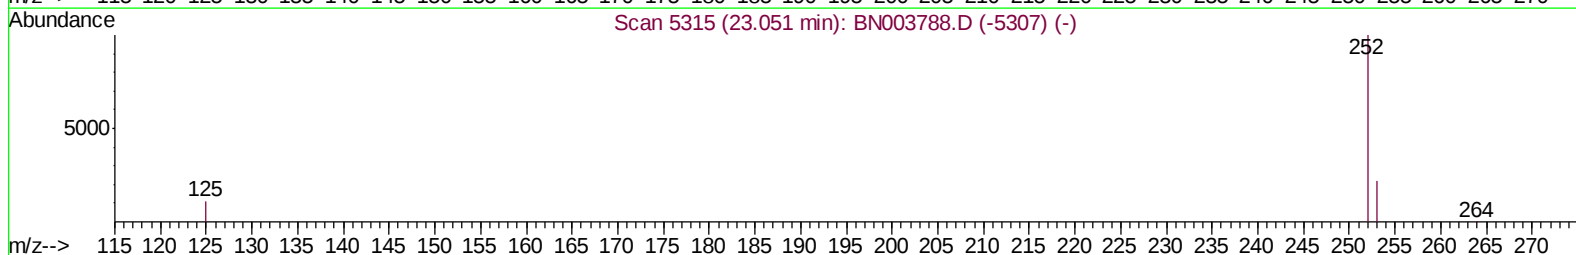
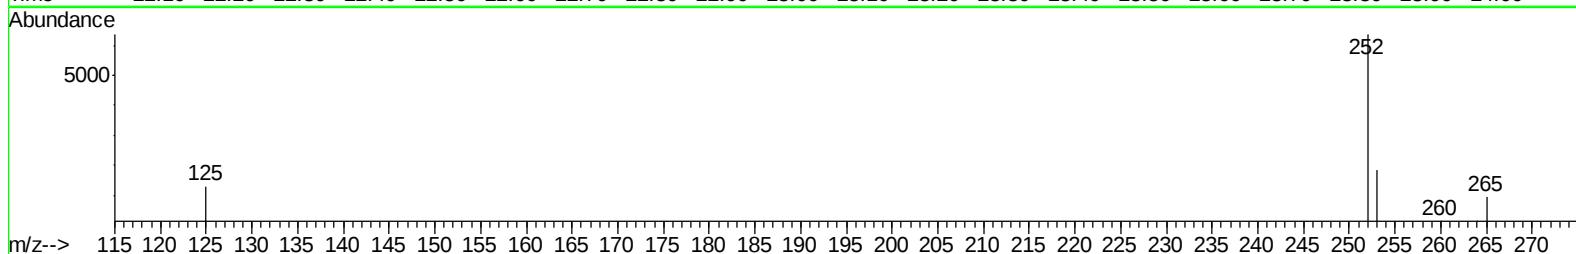


Data File : BN003792.D
Acq On : 10 Dec 2018 23:34
Operator : JU/SJ
Sample : J6077-12DL 5X
Misc :
ALS Vial : 18 Sample Multiplier: 1

Quant Time: Dec 11 04:26:45 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 11 04:22:54 2018
Response via : Initial Calibration

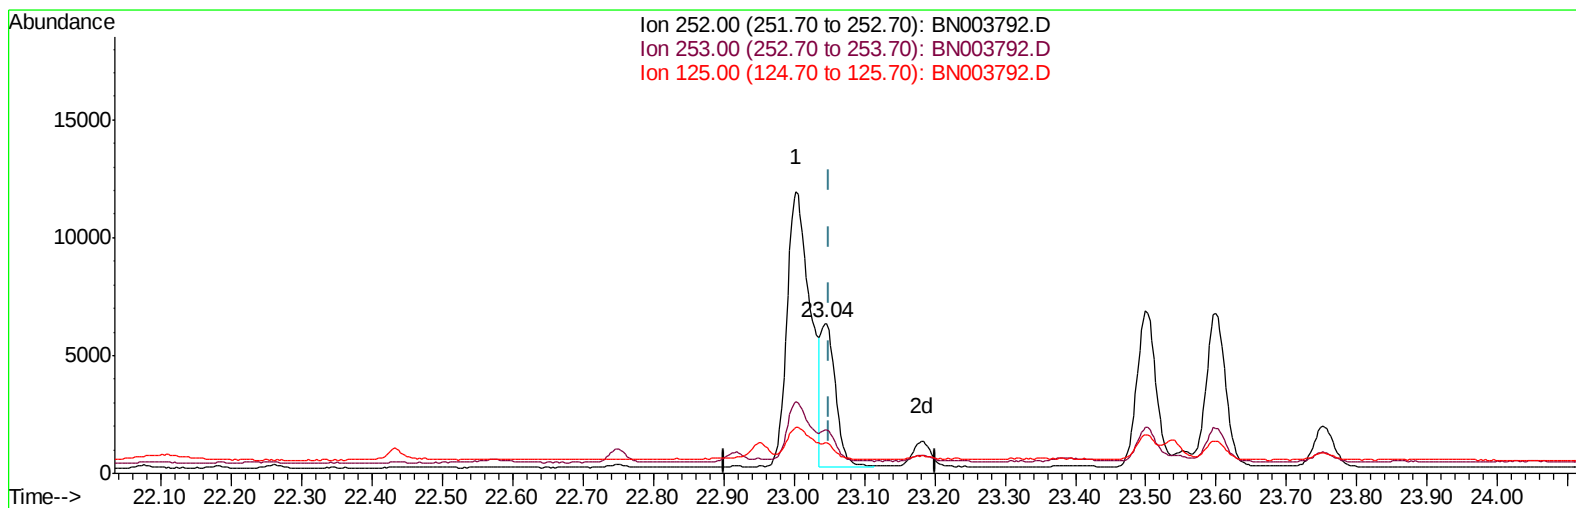

TIC: BN003792.D

(22) Benzo(k)fluoranthene

23.044min (-0.007) 0.10ng/ul m

response 9019

Ion	Exp%	Act%
252.00	100	100
253.00	23.10	29.00#
125.00	11.30	20.32#
0.00	0.00	0.00