
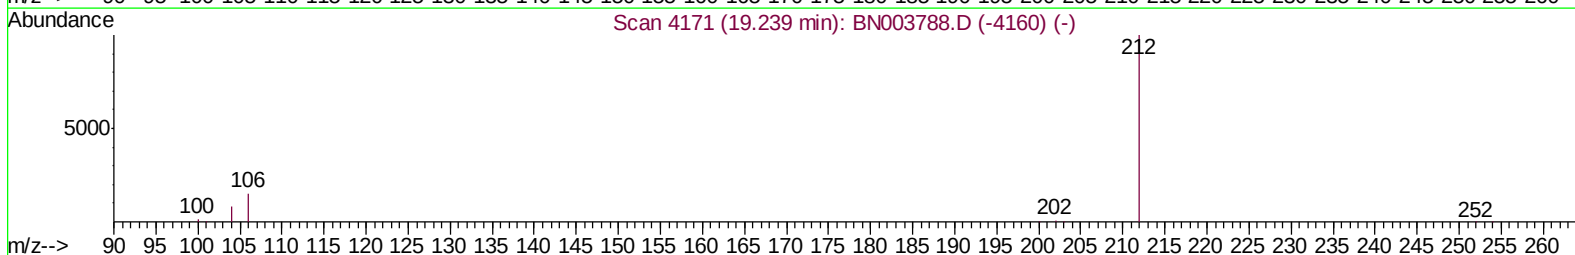
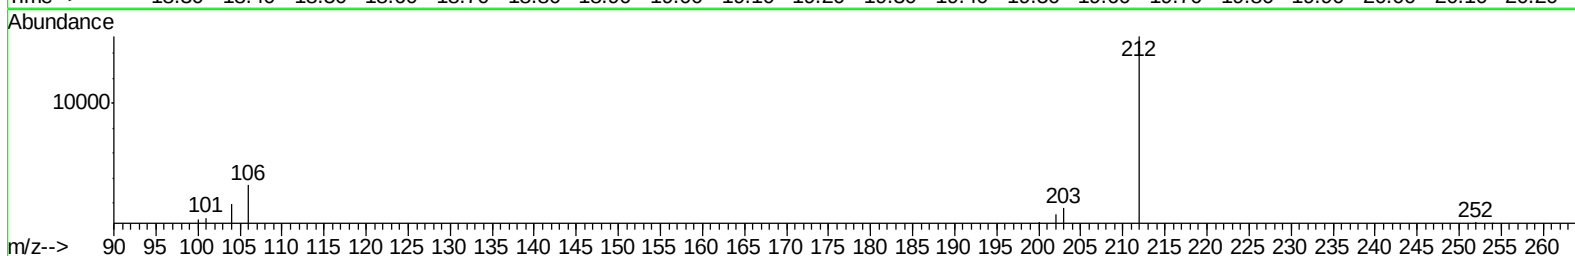


Data File : BN003793.D
Acq On : 11 Dec 2018 00:09
Operator : JU/SJ
Sample : J6077-14
Misc :
ALS Vial : 19 Sample Multiplier: 1

Quant Time: Dec 11 04:48:37 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 11 04:22:54 2018
Response via : Initial Calibration

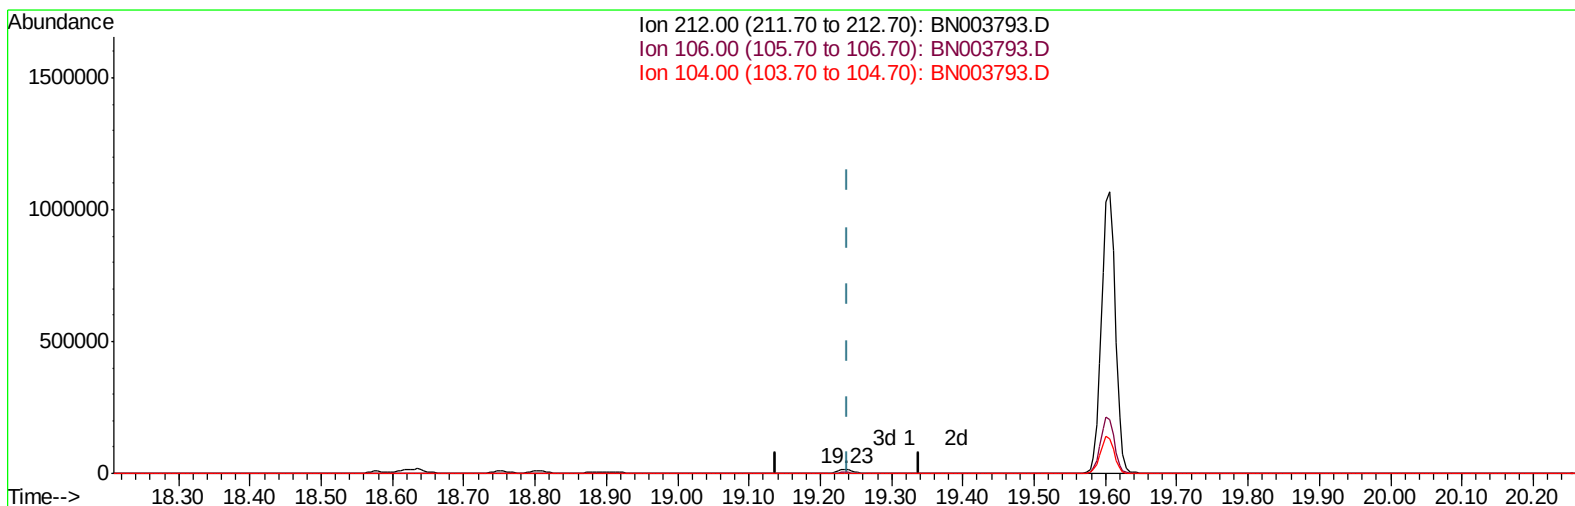

TIC: BN003793.D

(14) Fluoranthene-d10 (SURR)

19.234min (-0.005) 0.26ng/ul m

response 21479

Ion	Exp%	Act%
212.00	100	100
106.00	14.20	0.83#
104.00	8.00	1.82#
0.00	0.00	0.00