
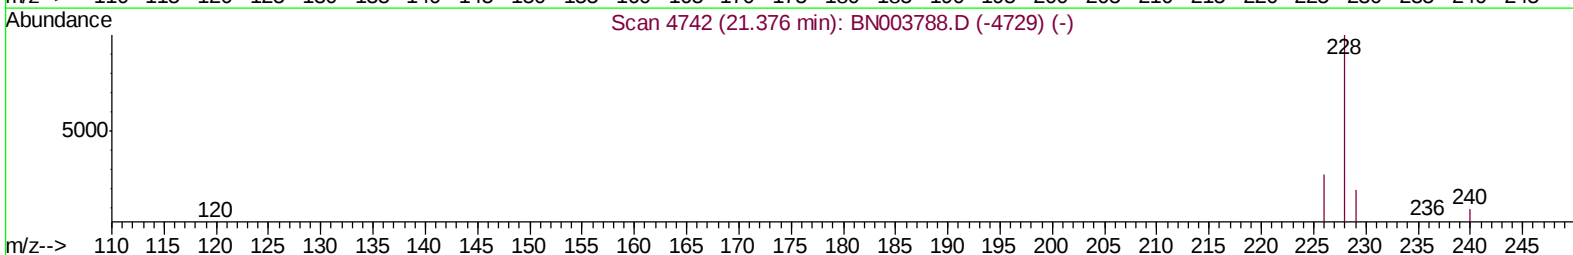
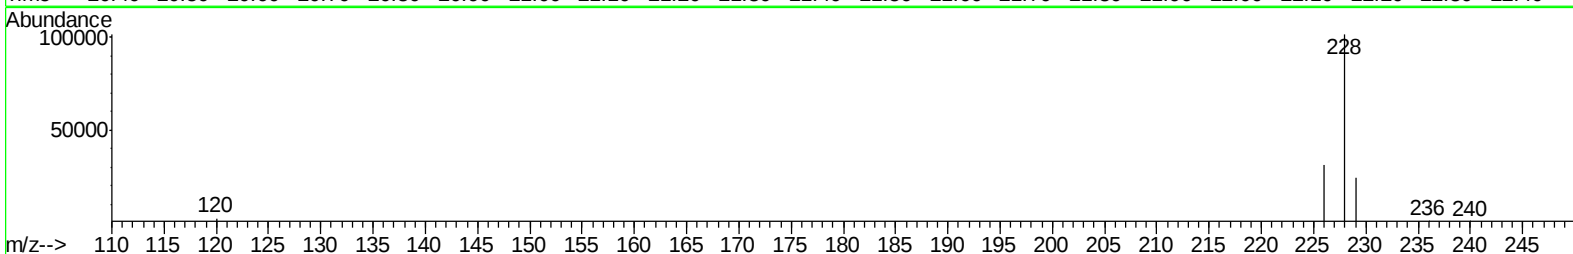


Data File : BN003793.D  
Acq On : 11 Dec 2018 00:09  
Operator : JU/SJ  
Sample : J6077-14  
Misc :  
ALS Vial : 19 Sample Multiplier: 1

Quant Time: Dec 11 04:50:05 2018  
Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_N\METHODS\SOM-EPA-SIM-BN111918.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Tue Dec 11 04:22:54 2018  
Response via : Initial Calibration

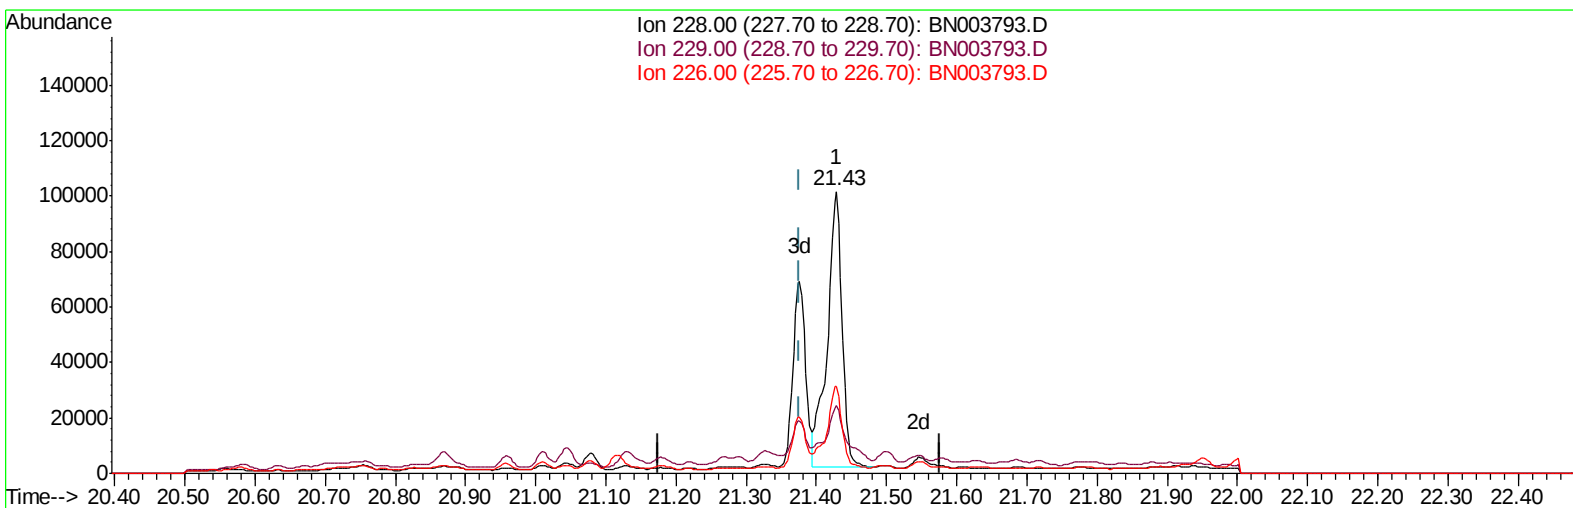

TIC: BN003793.D

(18) Benzo(a)anthracene  
21.429min (+0.052) 2.33ng/ul  
response 146045

| Ion    | Exp%  | Act%   |
|--------|-------|--------|
| 228.00 | 100   | 100    |
| 229.00 | 19.50 | 24.14# |
| 226.00 | 26.40 | 30.96  |
| 0.00   | 0.00  | 0.00   |