
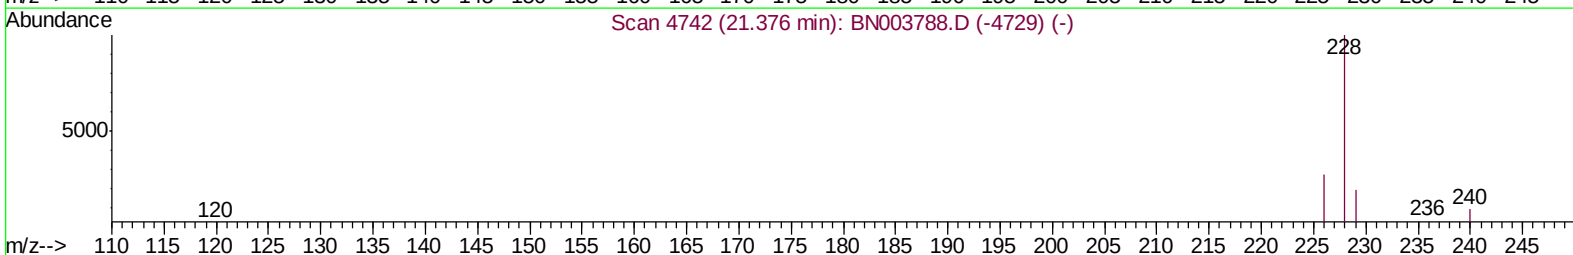
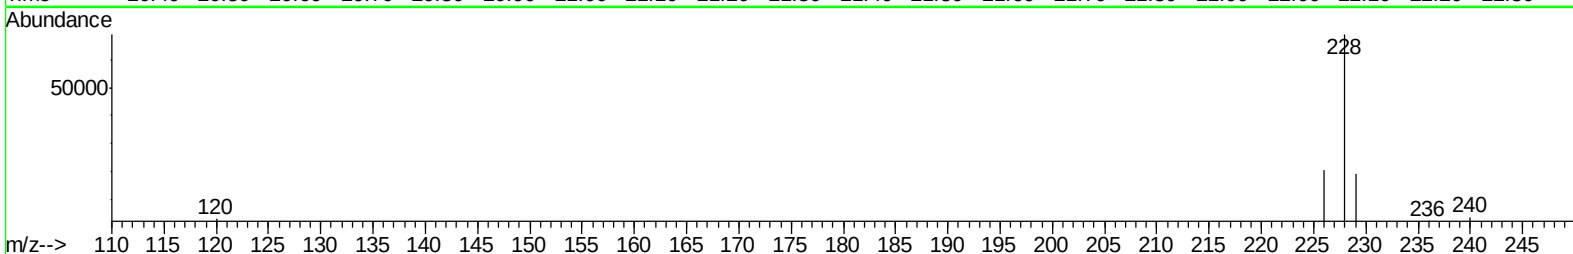


Data File : BN003793.D
Acq On : 11 Dec 2018 00:09
Operator : JU/SJ
Sample : J6077-14
Misc :
ALS Vial : 19 Sample Multiplier: 1

Quant Time: Dec 11 04:50:05 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 11 04:22:54 2018
Response via : Initial Calibration

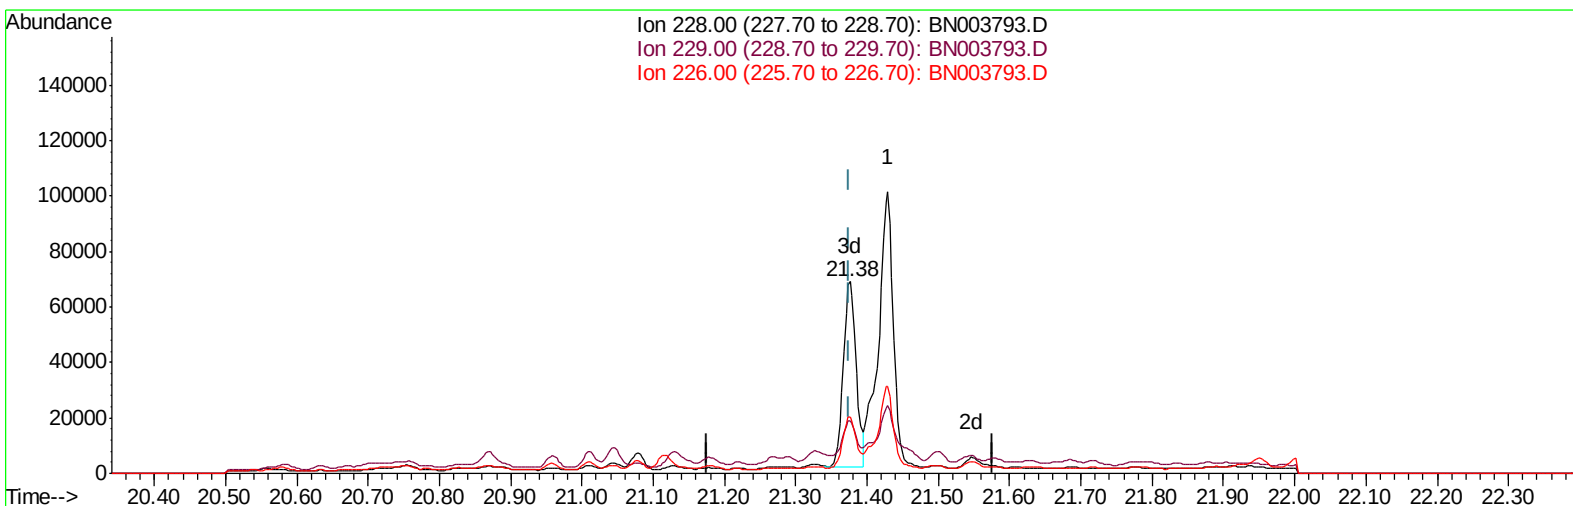

TIC: BN003793.D

(18) Benzo(a)anthracene
21.376min (-0.000) 1.34ng/ul m
response 83854

Ion	Exp%	Act%
228.00	100	100
229.00	19.50	27.52#
226.00	26.40	29.36
0.00	0.00	0.00