
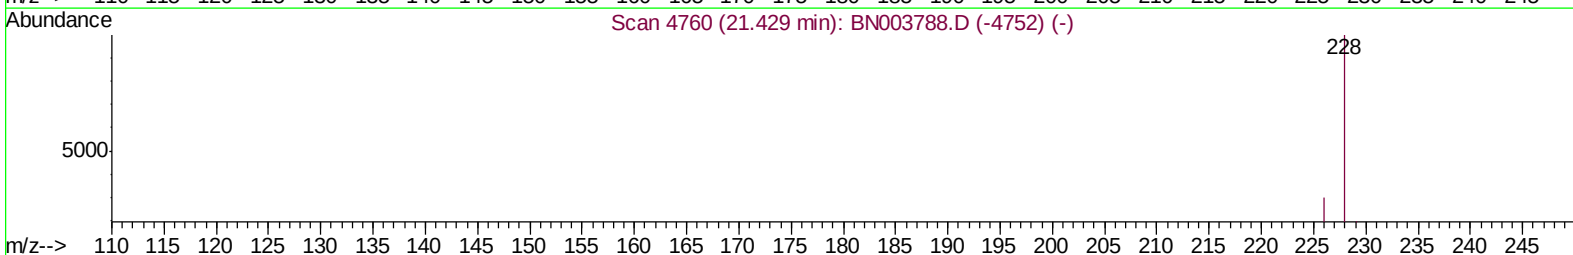
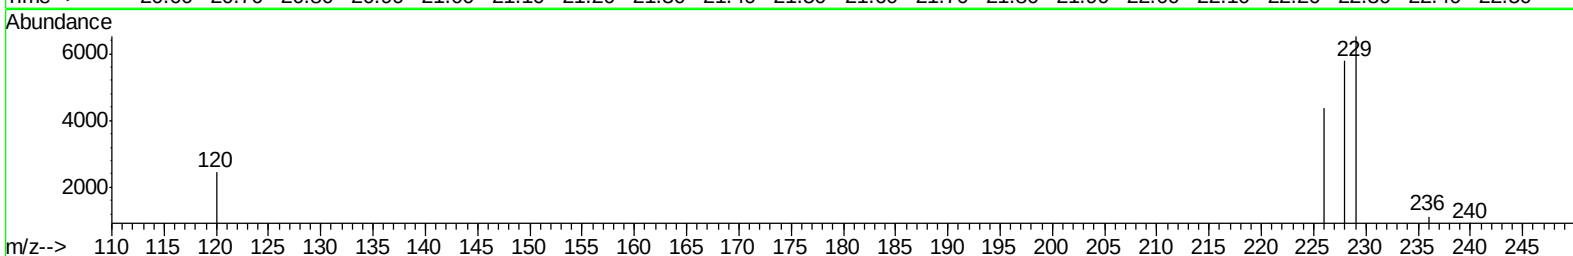


Data File : BN003793.D
Acq On : 11 Dec 2018 00:09
Operator : JU/SJ
Sample : J6077-14
Misc :
ALS Vial : 19 Sample Multiplier: 1

Quant Time: Dec 11 04:50:05 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 11 04:22:54 2018
Response via : Initial Calibration

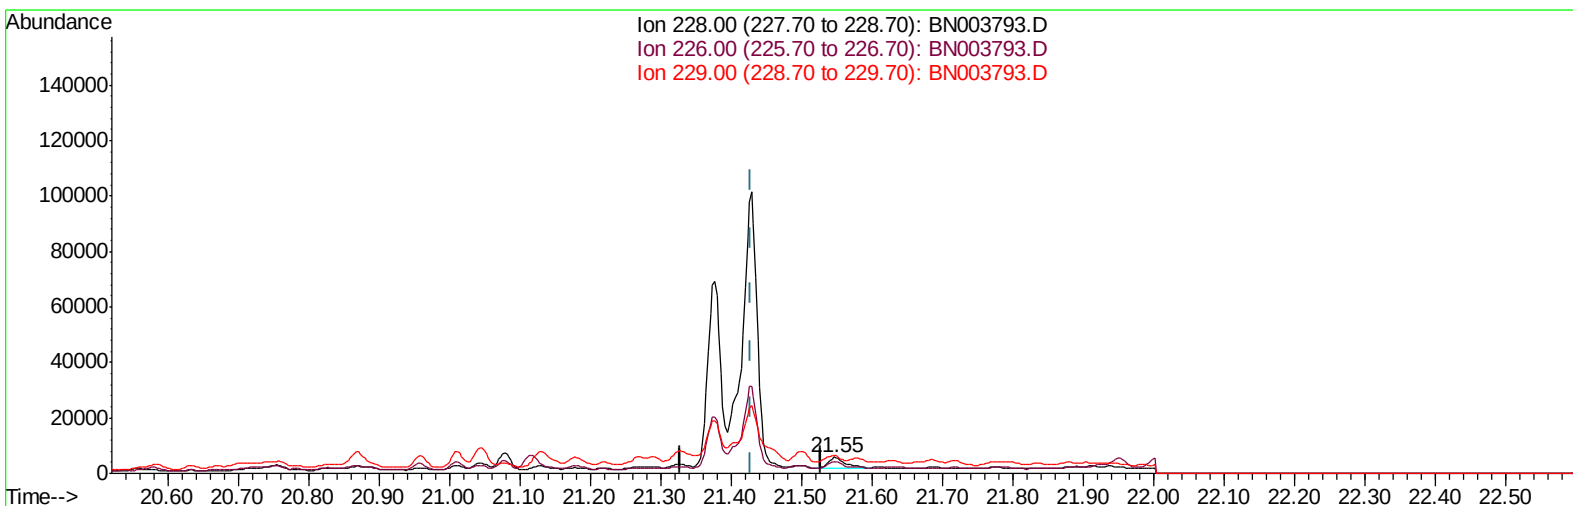

TIC: BN003793.D

(19) Chrysene

21.546min (+0.117) 0.10ng/ul

response 7142

Ion	Exp%	Act%
228.00	100	100
226.00	30.00	75.60#
229.00	19.60	112.60#
0.00	0.00	0.00