
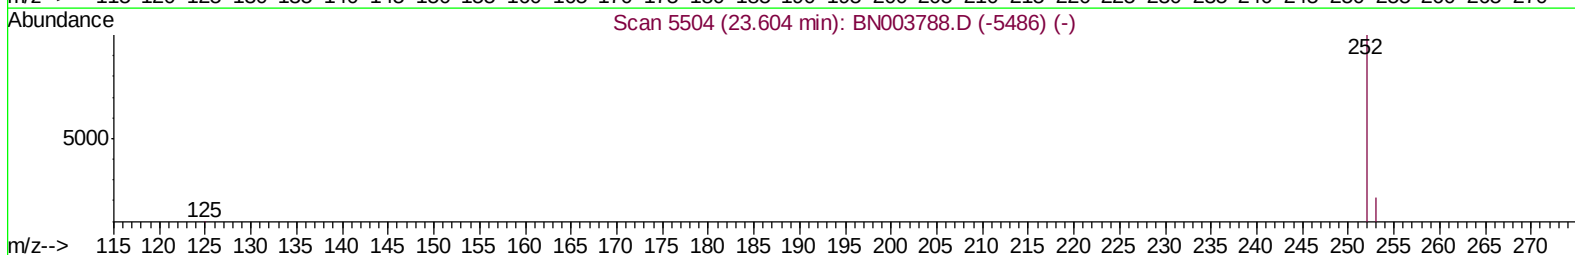
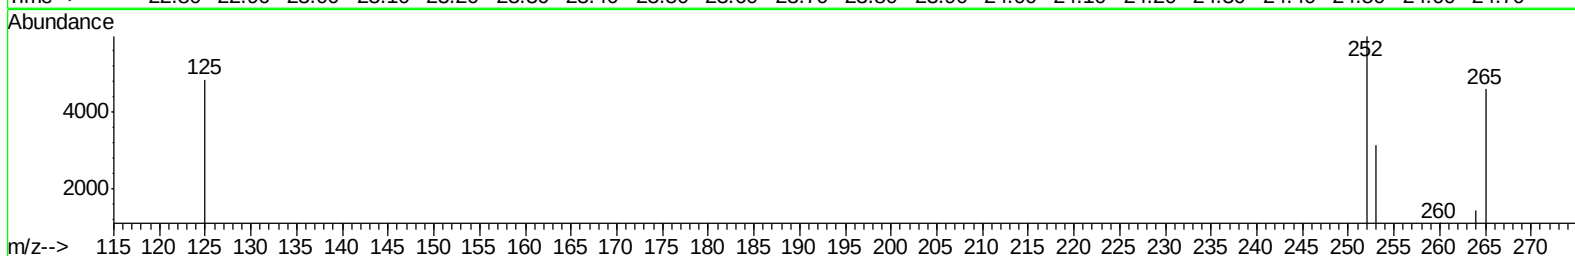


Data File : BN003793.D
Acq On : 11 Dec 2018 00:09
Operator : JU/SJ
Sample : J6077-14
Misc :
ALS Vial : 19 Sample Multiplier: 1

Quant Time: Dec 11 04:51:31 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 11 04:22:54 2018
Response via : Initial Calibration

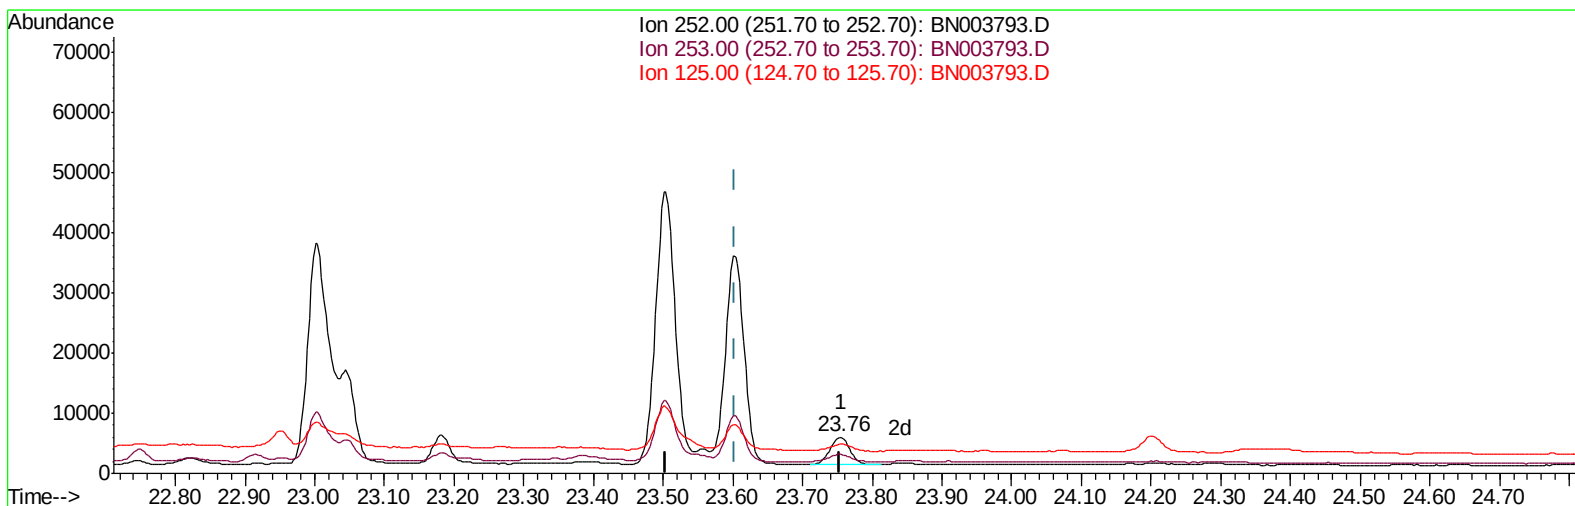

TIC: BN003793.D

(23) Benzo(a)pyrene (C)
23.755min (+0.152) 0.15ng/ul
response 9191

Ion	Exp%	Act%
252.00	100	100
253.00	23.70	52.43#
125.00	12.80	81.13#
0.00	0.00	0.00