
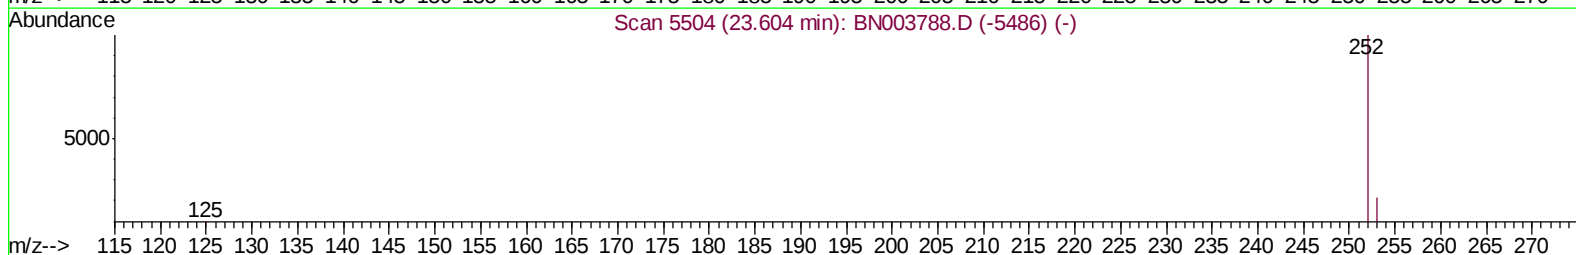
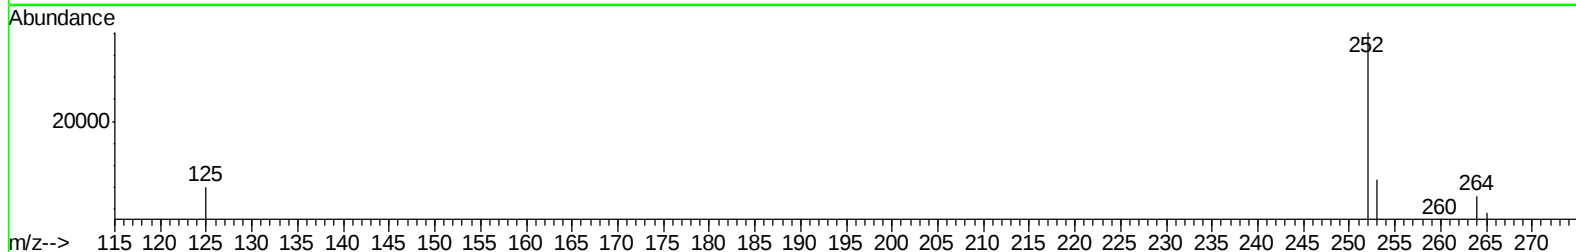


Data File : BN003793.D
Acq On : 11 Dec 2018 00:09
Operator : JU/SJ
Sample : J6077-14
Misc :
ALS Vial : 19 Sample Multiplier: 1

Quant Time: Dec 11 04:51:31 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 11 04:22:54 2018
Response via : Initial Calibration

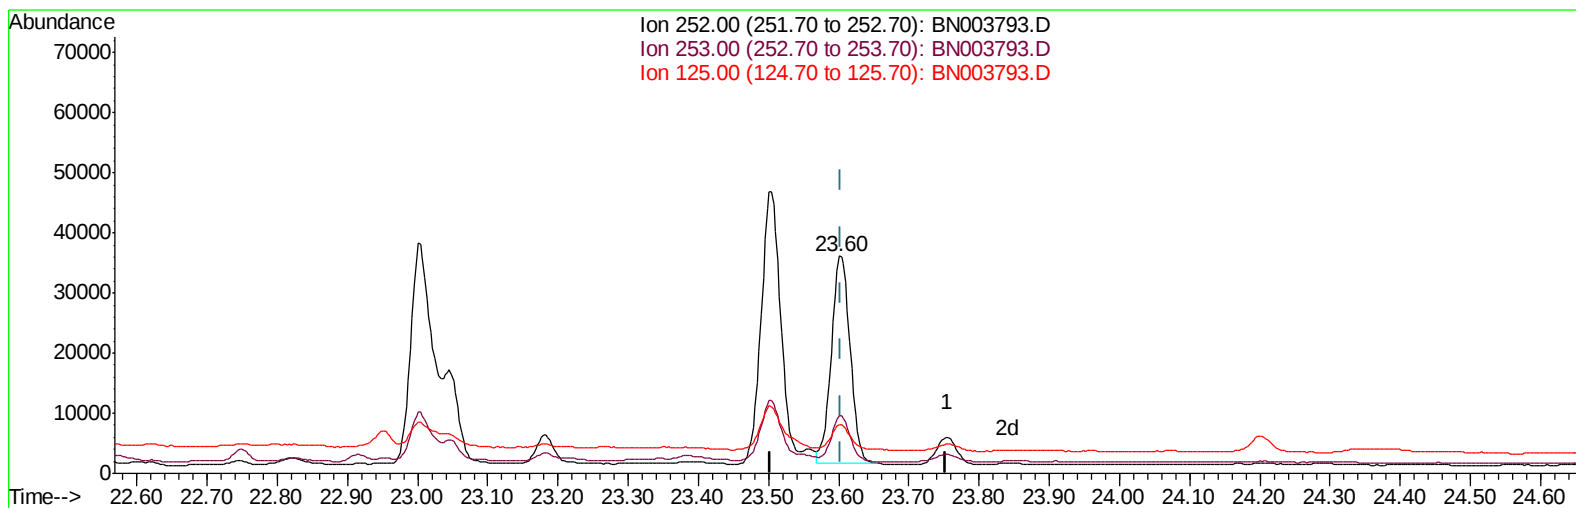

TIC: BN003793.D

(23) Benzo(a)pyrene (C)

23.601min (-0.003) 1.08ng/ul m

response 64316

Ion	Exp%	Act%
252.00	100	100
253.00	23.70	26.34
125.00	12.80	22.56#
0.00	0.00	0.00