
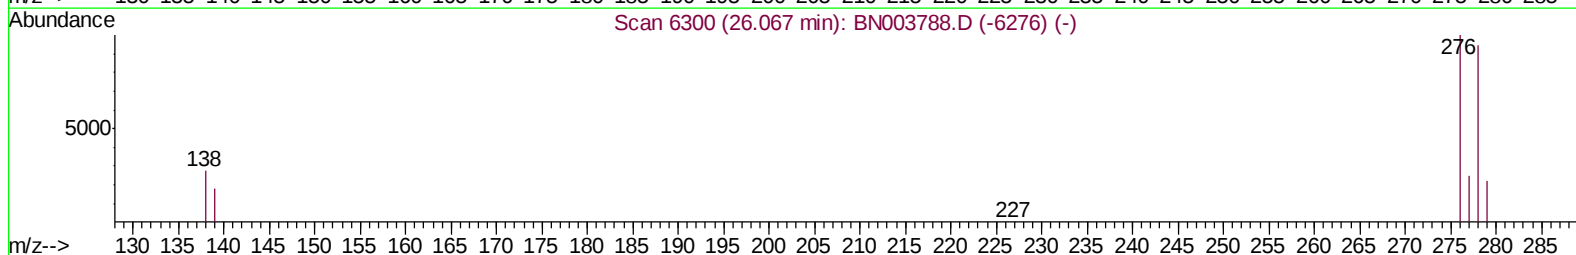
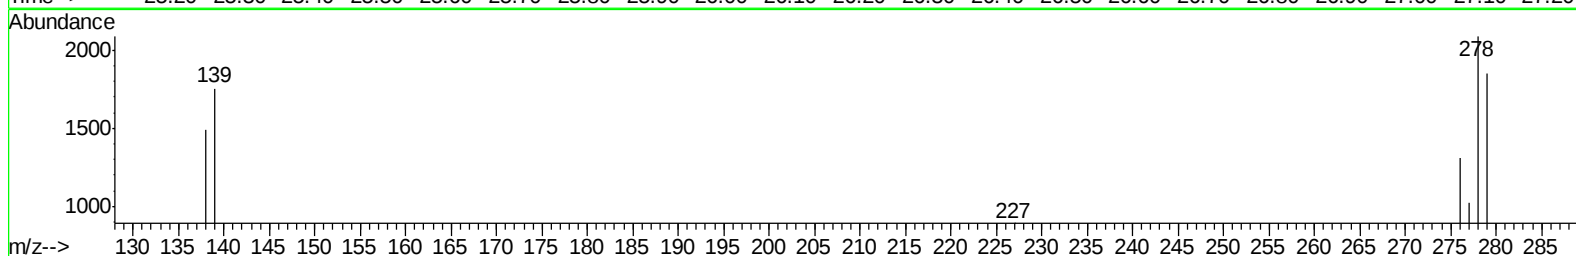


Data File : BN003793.D
Acq On : 11 Dec 2018 00:09
Operator : JU/SJ
Sample : J6077-14
Misc :
ALS Vial : 19 Sample Multiplier: 1

Quant Time: Dec 11 04:51:31 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 11 04:22:54 2018
Response via : Initial Calibration

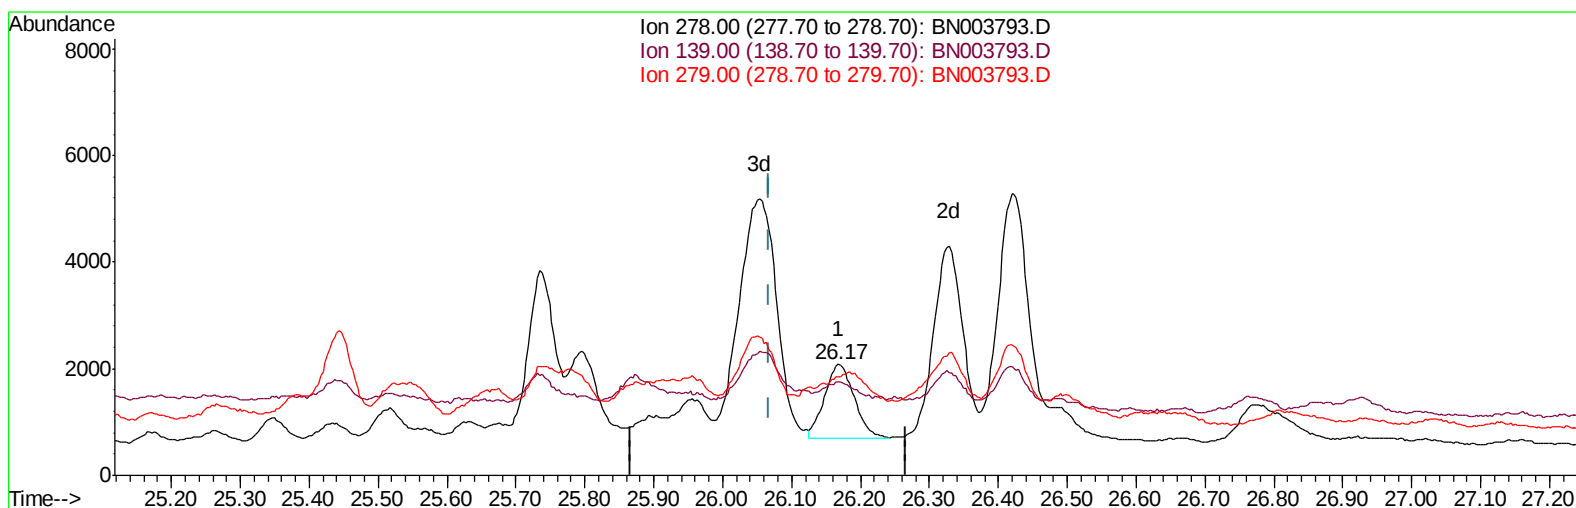

TIC: BN003793.D

(25) Dibenzo(a,h)anthracene

26.168min (+0.101) 0.08ng/ul

response 4183

Ion	Exp%	Act%
278.00	100	100
139.00	17.80	83.94#
279.00	24.70	88.64#
0.00	0.00	0.00