
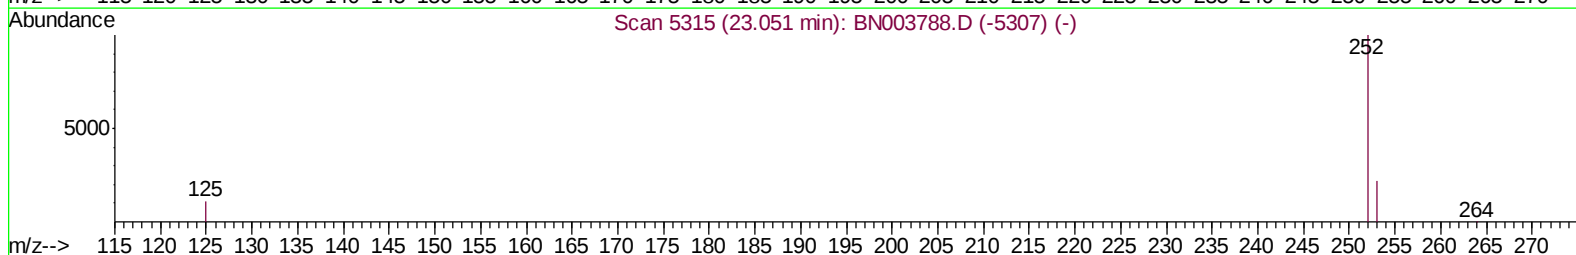
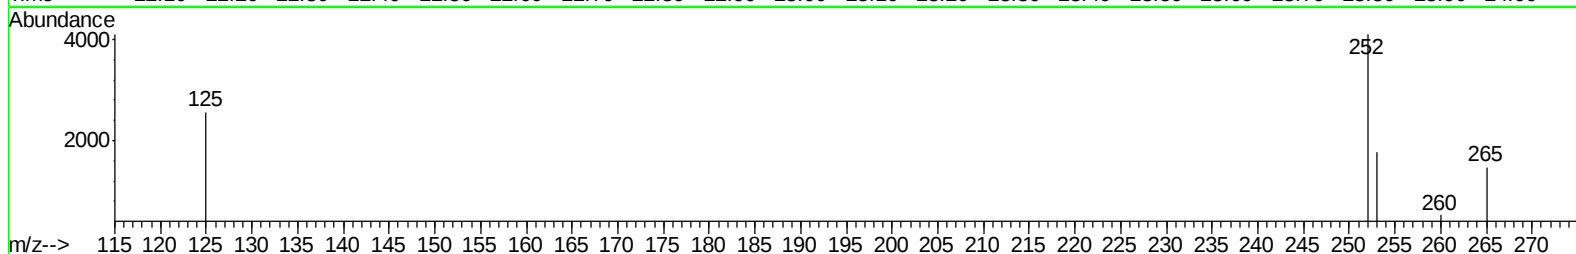


Data File : BN003794.D
Acq On : 11 Dec 2018 00:44
Operator : JU/SJ
Sample : J6077-14DL 5X
Misc :
ALS Vial : 20 Sample Multiplier: 1

Quant Time: Dec 11 04:27:04 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 11 04:22:54 2018
Response via : Initial Calibration

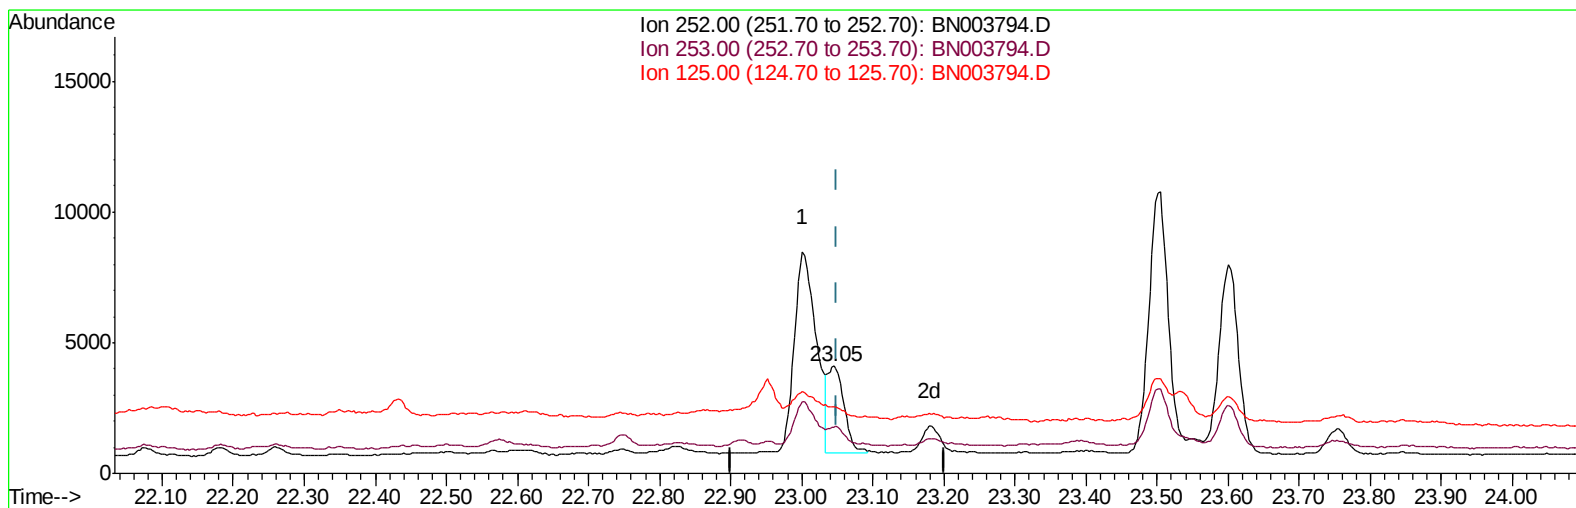

TIC: BN003794.D

(22) Benzo(k)fluoranthene

23.045min (-0.006) 0.07ng/ul m

response 5278

Ion	Exp%	Act%
252.00	100	100
253.00	23.10	43.29#
125.00	11.30	62.52#
0.00	0.00	0.00