
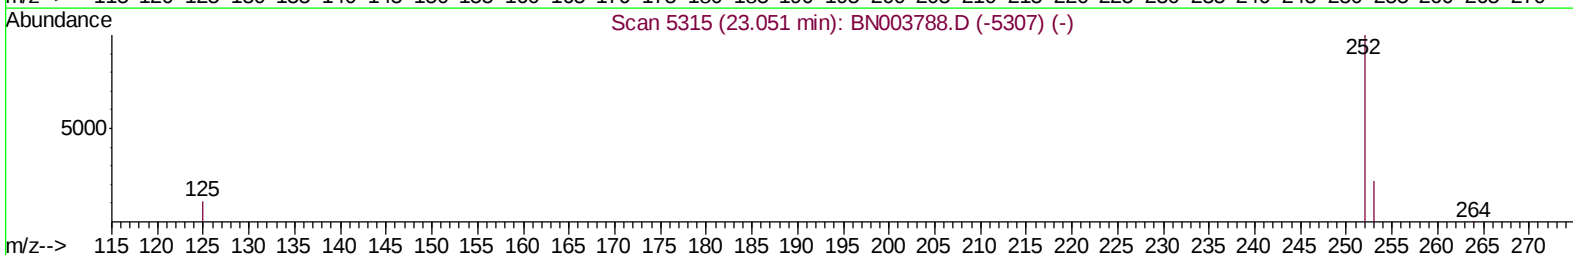
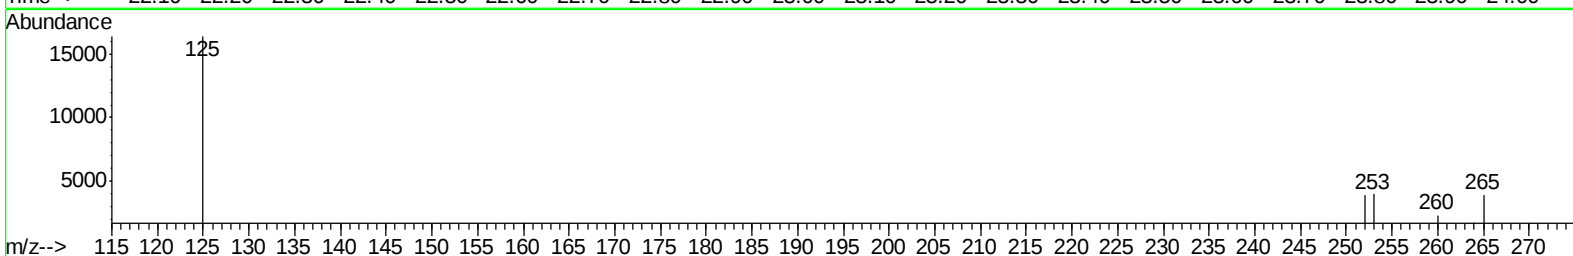


Data File : BN003796.D
Acq On : 11 Dec 2018 01:54
Operator : JU/SJ
Sample : J6077-15DL 5X
Misc :
ALS Vial : 22 Sample Multiplier: 1

Quant Time: Dec 11 05:40:20 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 11 04:22:54 2018
Response via : Initial Calibration

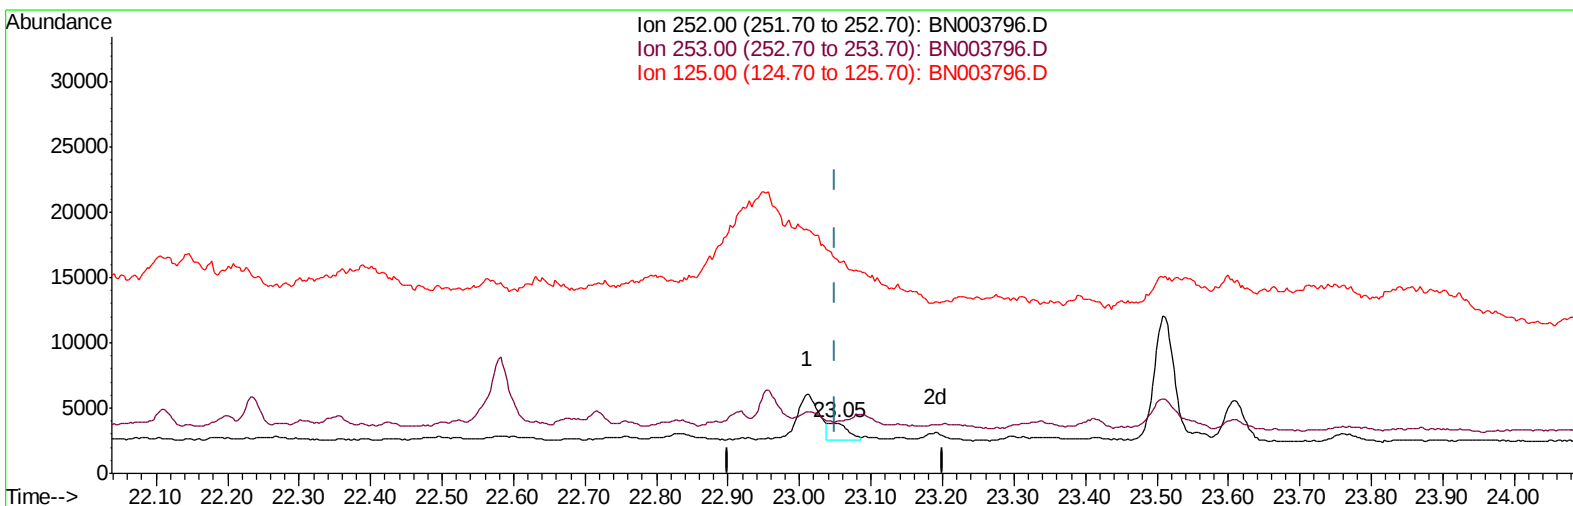

TIC: BN003796.D

(22) Benzo(k)fluoranthene

23.053min (+0.002) 0.03ng/ul m

response 2360

Ion	Exp%	Act%
252.00	100	100
253.00	23.10	103.26#
125.00	11.30	424.44#
0.00	0.00	0.00