
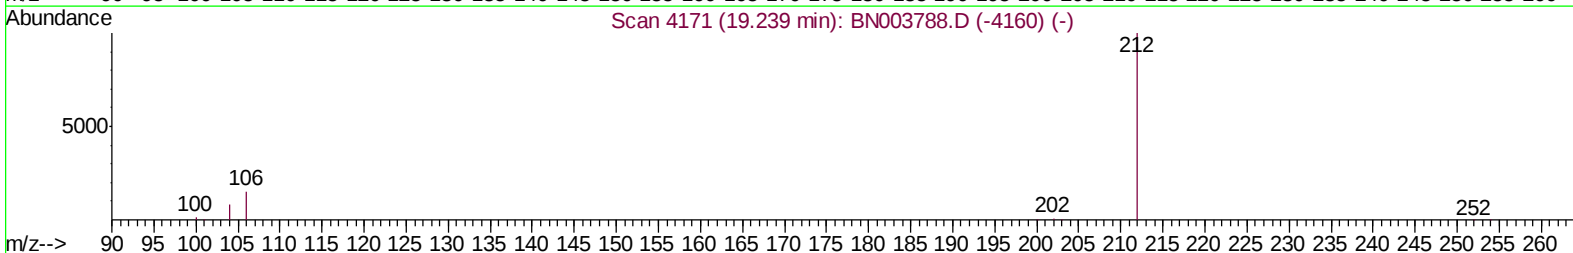
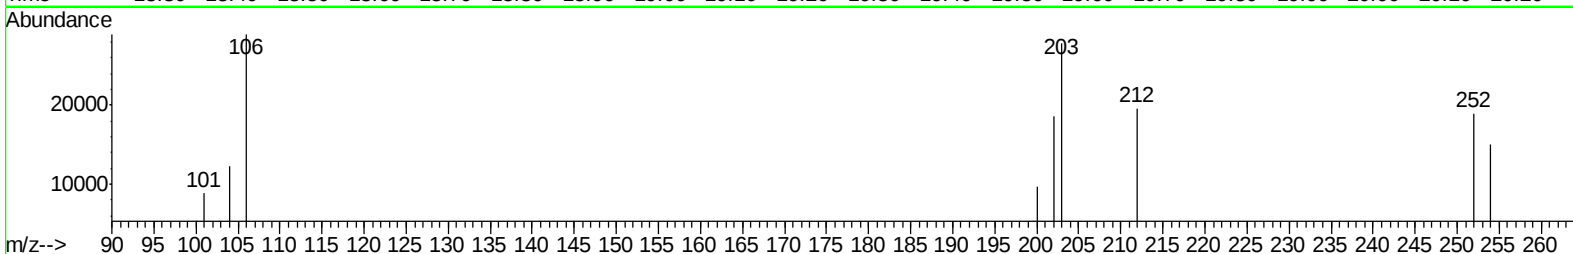


Data File : BN003797.D
Acq On : 11 Dec 2018 02:29
Operator : JU/SJ
Sample : J6077-16
Misc :
ALS Vial : 23 Sample Multiplier: 1

Quant Time: Dec 11 05:43:21 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 11 04:22:54 2018
Response via : Initial Calibration

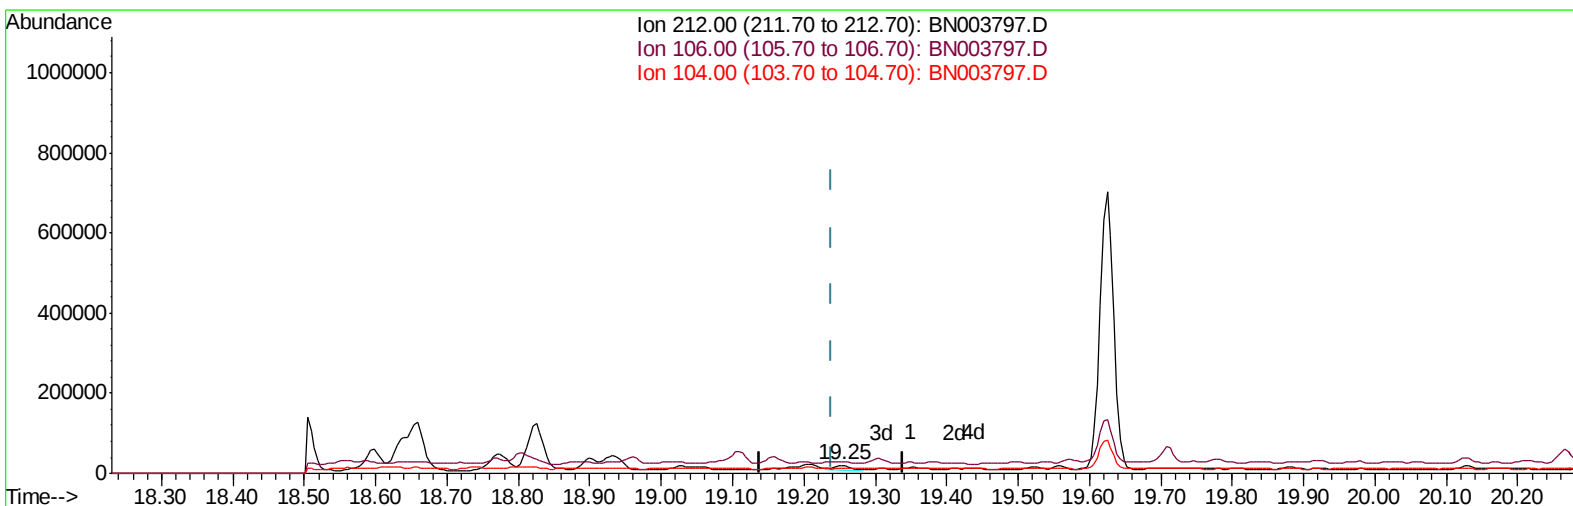

TIC: BN003797.D

(14) Fluoranthene-d10 (SURR)

19.253min (+0.014) 0.28ng/ul m

response 18452

Ion	Exp%	Act%
212.00	100	100
106.00	14.20	18.13#
104.00	8.00	22.12#
0.00	0.00	0.00