
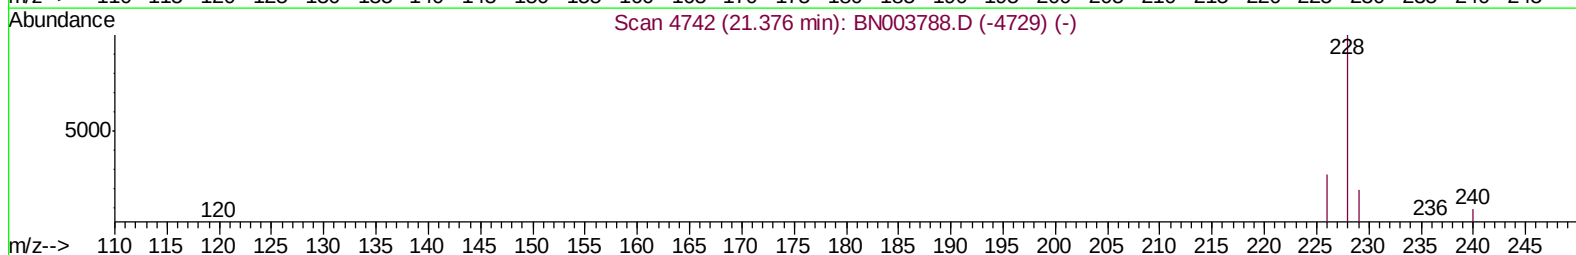
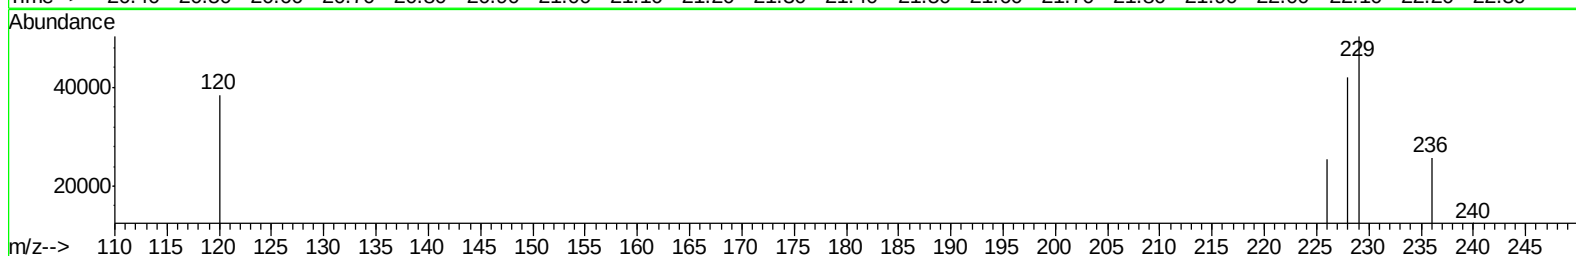


Data File : BN003797.D
Acq On : 11 Dec 2018 02:29
Operator : JU/SJ
Sample : J6077-16
Misc :
ALS Vial : 23 Sample Multiplier: 1

Quant Time: Dec 11 05:45:29 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 11 04:22:54 2018
Response via : Initial Calibration

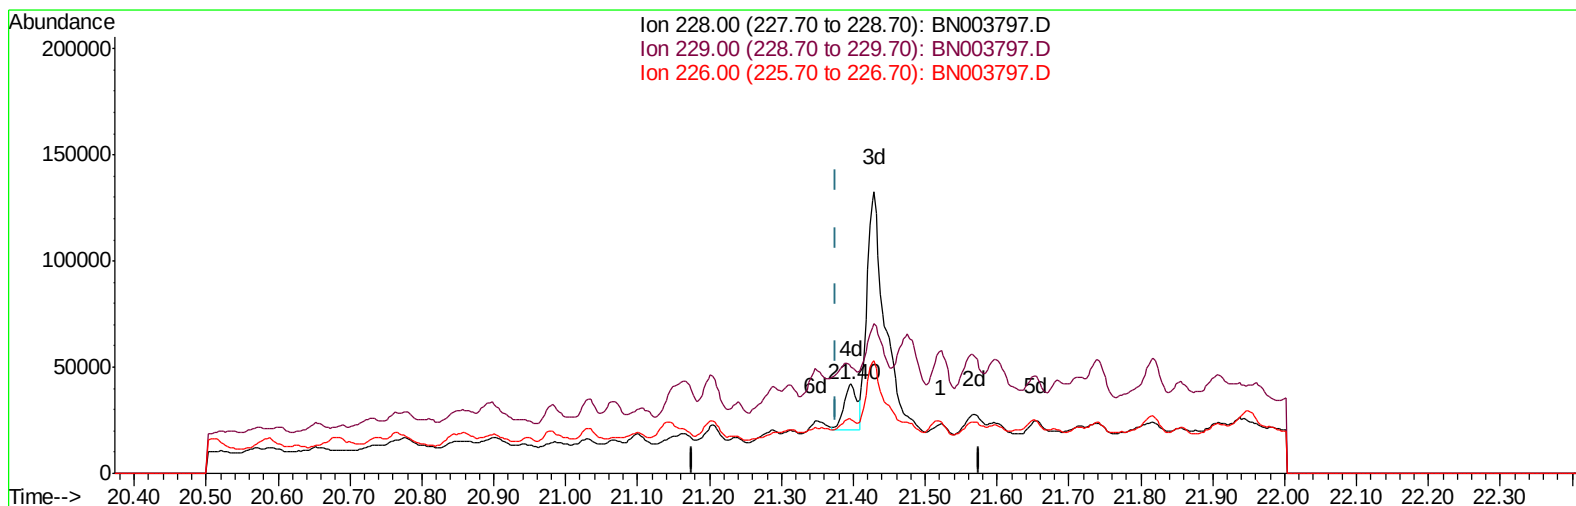

TIC: BN003797.D

(18) Benzo(a)anthracene

21.397min (+0.021) 0.62ng/ul m

response 28011

Ion	Exp%	Act%
228.00	100	100
229.00	19.50	119.87#
226.00	26.40	60.59#
0.00	0.00	0.00