
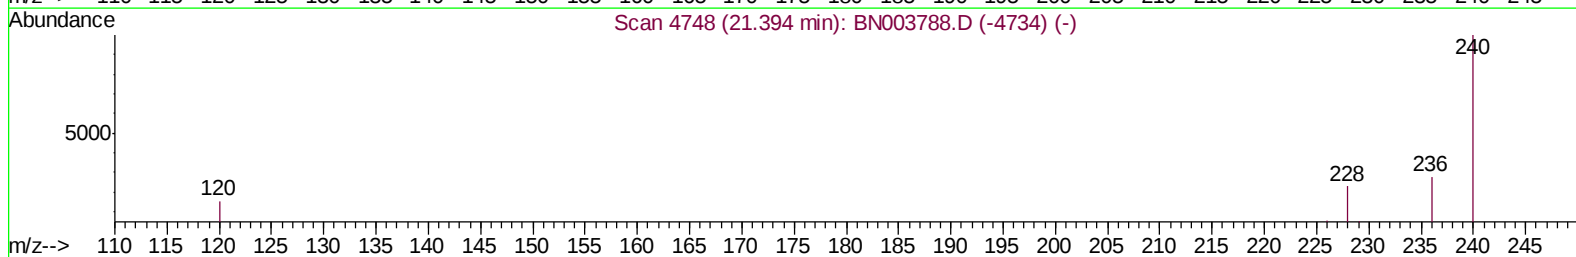
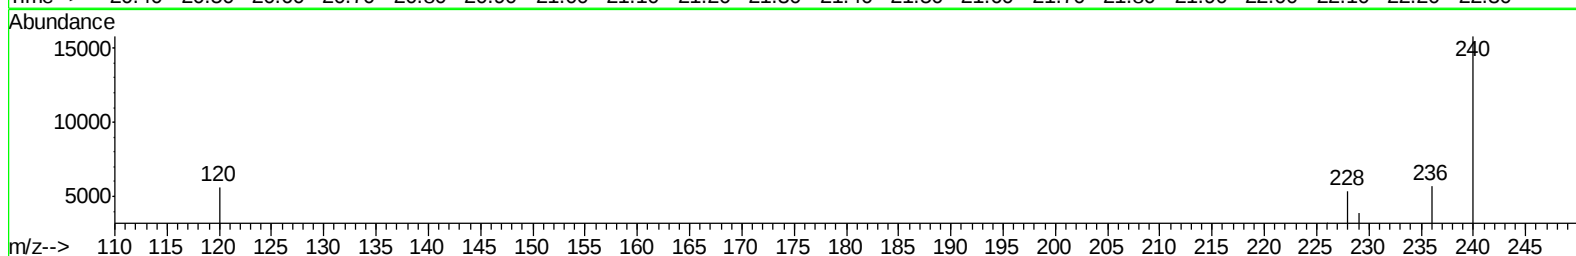


Data File : BN003799.D
Acq On : 11 Dec 2018 03:39
Operator : JU/SJ
Sample : J6077-18
Misc :
ALS Vial : 25 Sample Multiplier: 1

Quant Time: Dec 11 05:54:26 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 11 04:22:54 2018
Response via : Initial Calibration

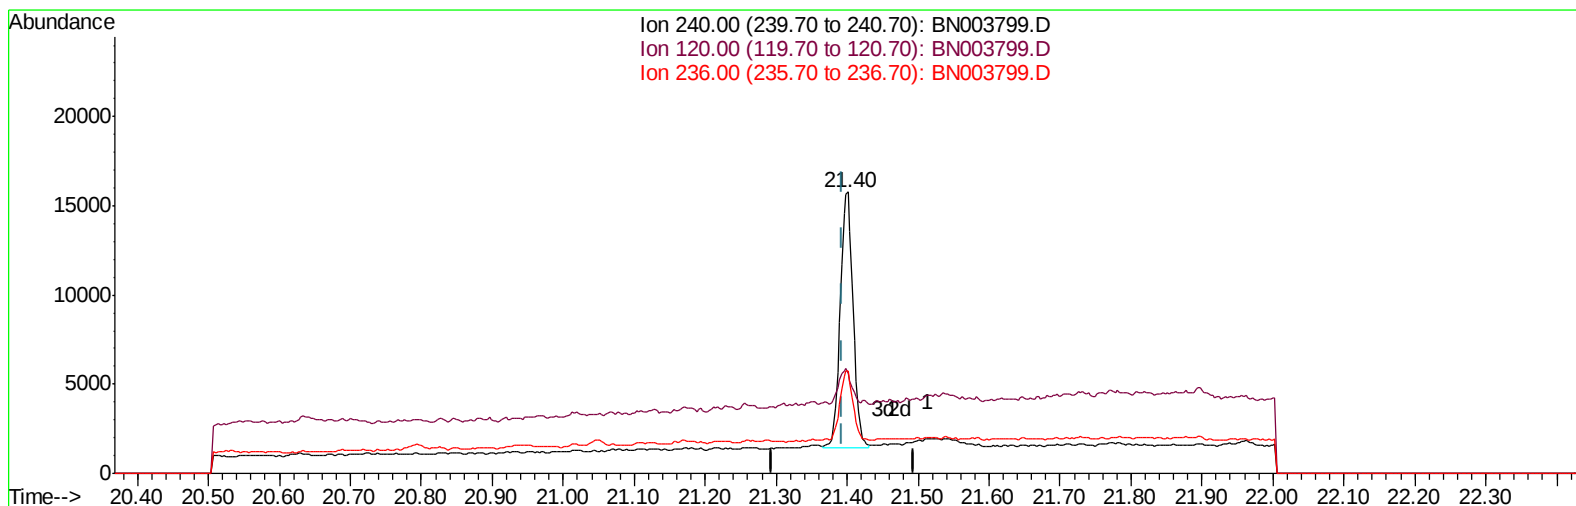

TIC: BN003799.D

(16) Chrysene-d12 (I)

21.401min (+0.007) 0.40ng/ul m

response 17940

Ion	Exp%	Act%
240.00	100	100
120.00	14.00	35.61#
236.00	27.60	36.30#
0.00	0.00	0.00