
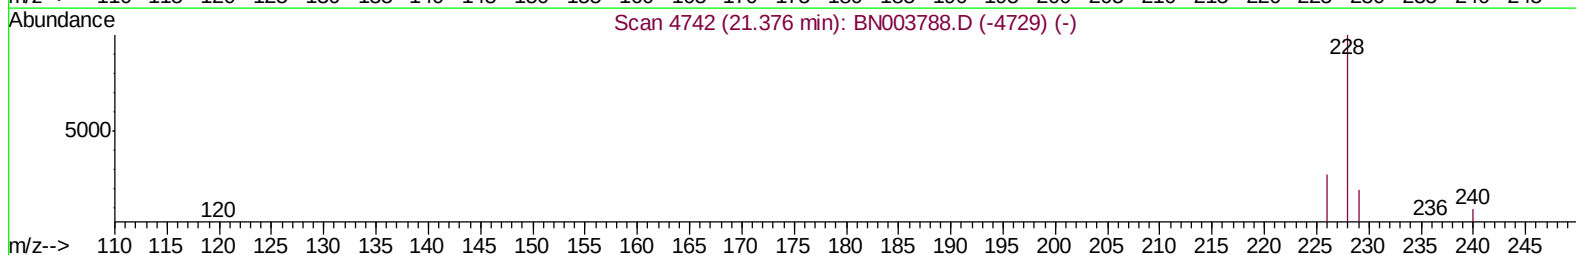
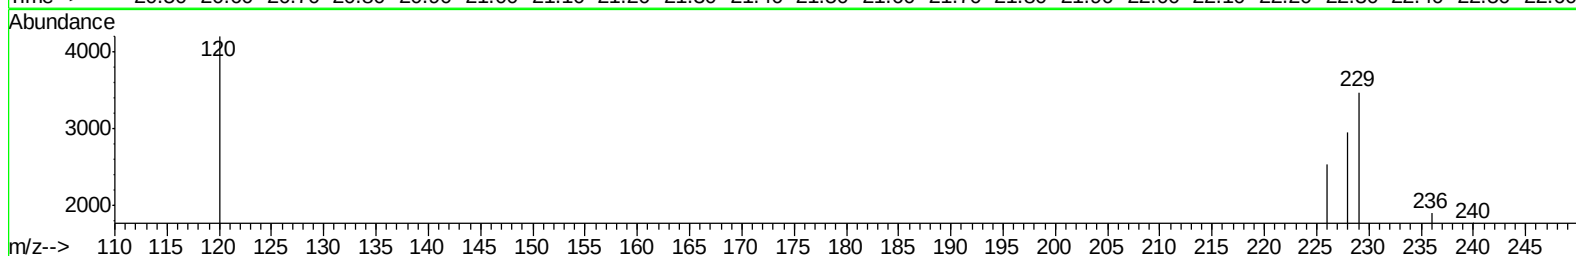


Data File : BN003799.D
Acq On : 11 Dec 2018 03:39
Operator : JU/SJ
Sample : J6077-18
Misc :
ALS Vial : 25 Sample Multiplier: 1

Quant Time: Dec 11 05:57:09 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 11 04:22:54 2018
Response via : Initial Calibration

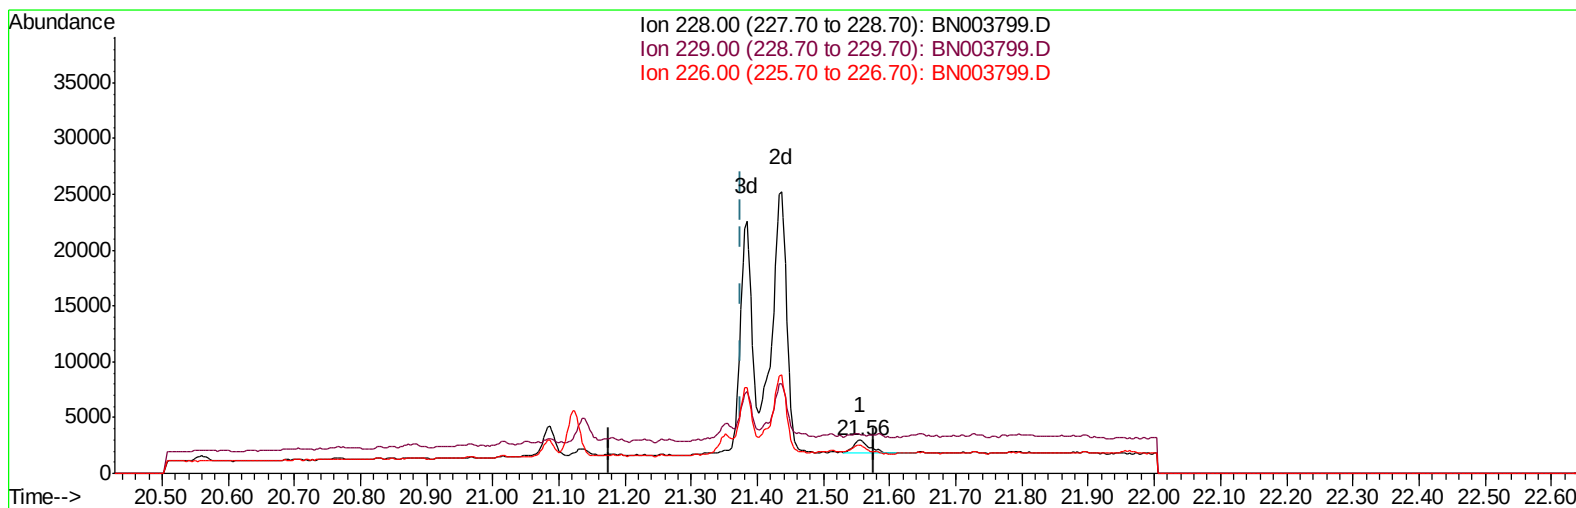

TIC: BN003799.D

(18) Benzo(a)anthracene
21.556min (+0.180) 0.04ng/ul
response 2090

Ion	Exp%	Act%
228.00	100	100
229.00	19.50	117.28#
226.00	26.40	85.43#
0.00	0.00	0.00