
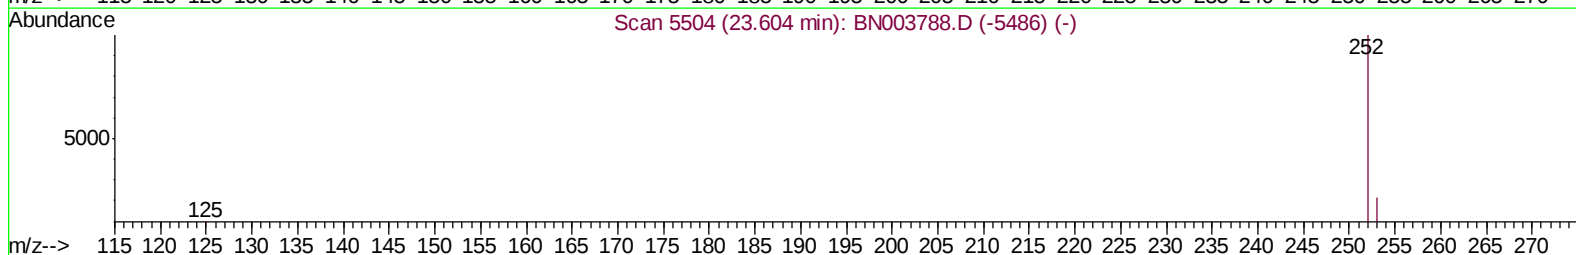
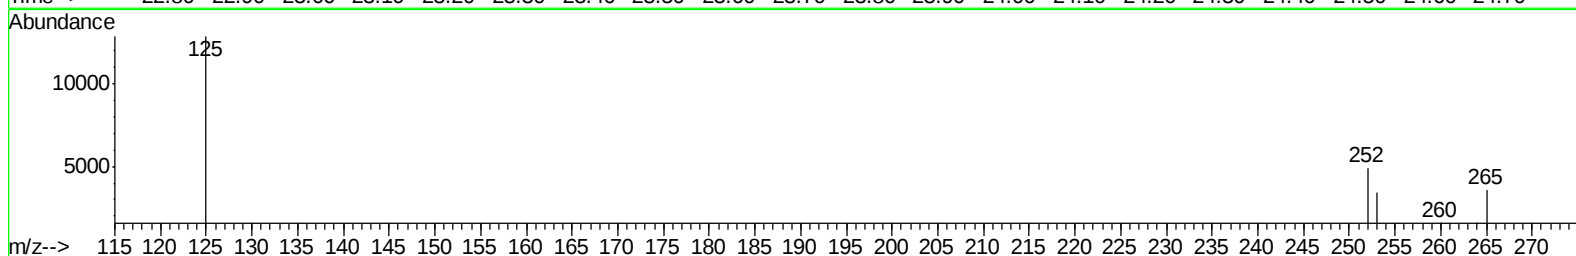


Data File : BN003799.D
Acq On : 11 Dec 2018 03:39
Operator : JU/SJ
Sample : J6077-18
Misc :
ALS Vial : 25 Sample Multiplier: 1

Quant Time: Dec 11 05:58:09 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 11 04:22:54 2018
Response via : Initial Calibration

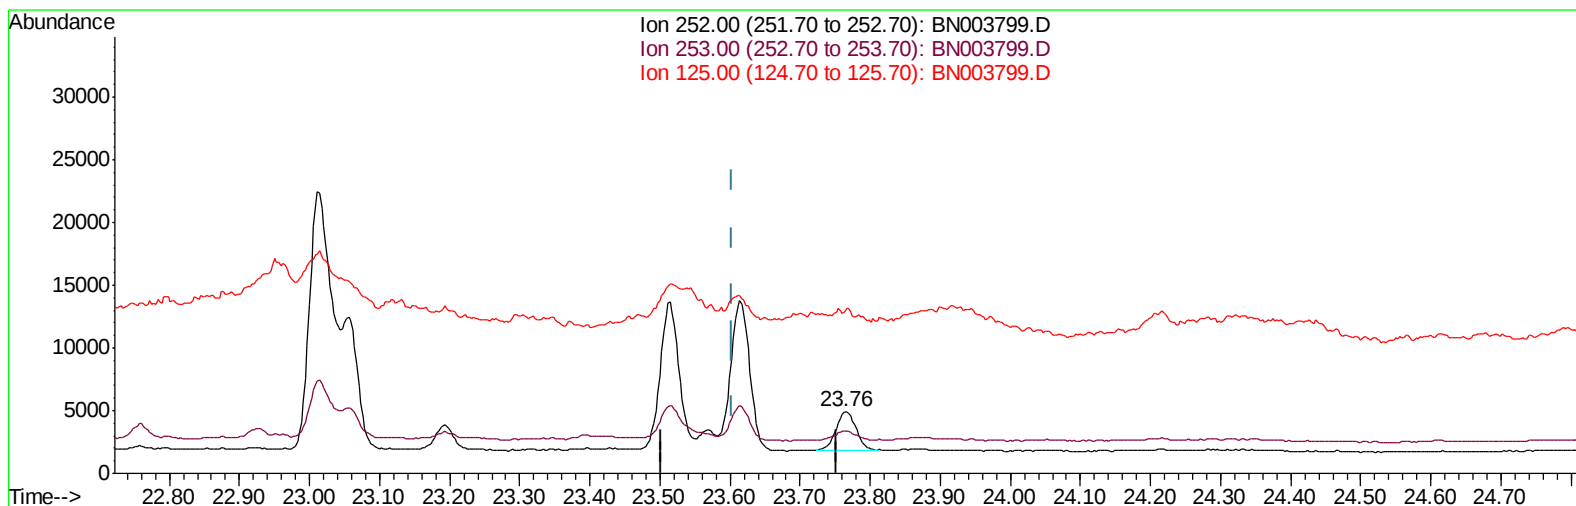

TIC: BN003799.D

(23) Benzo(a)pyrene (C)
23.763min (+0.159) 0.10ng/ul
response 6077

Ion	Exp%	Act%
252.00	100	100
253.00	23.70	68.99#
125.00	12.80	262.15#
0.00	0.00	0.00