
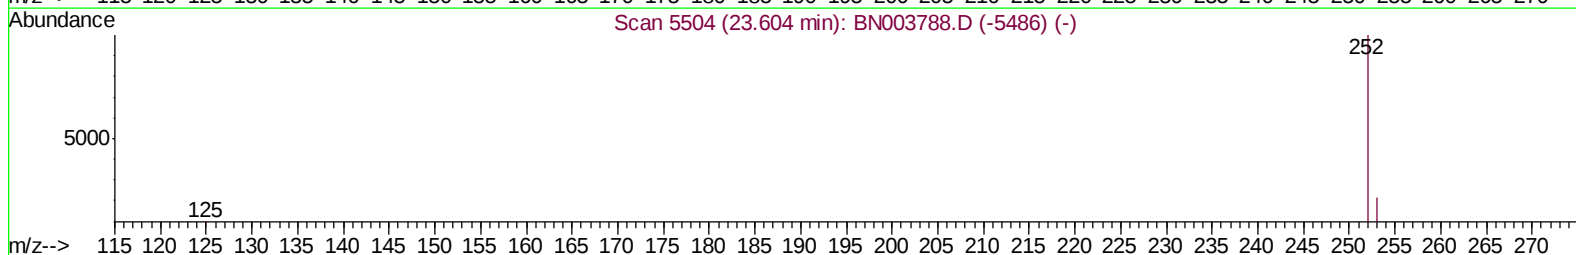
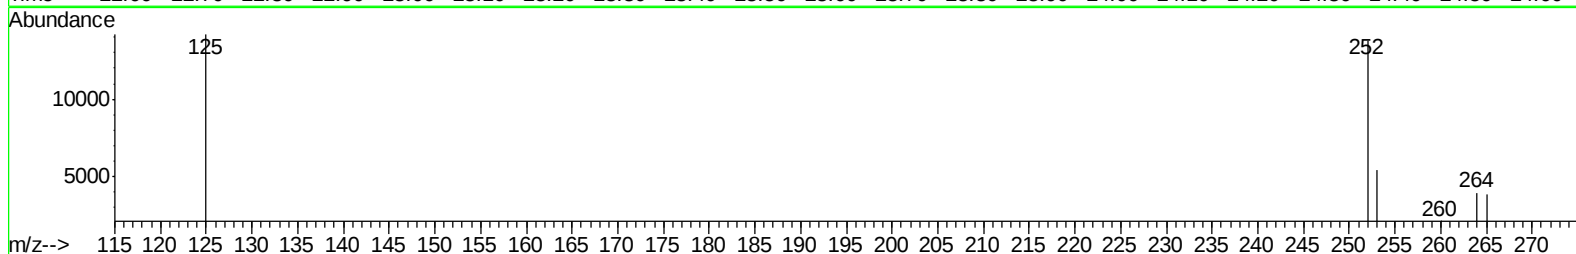


Data File : BN003799.D
Acq On : 11 Dec 2018 03:39
Operator : JU/SJ
Sample : J6077-18
Misc :
ALS Vial : 25 Sample Multiplier: 1

Quant Time: Dec 11 05:58:09 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 11 04:22:54 2018
Response via : Initial Calibration

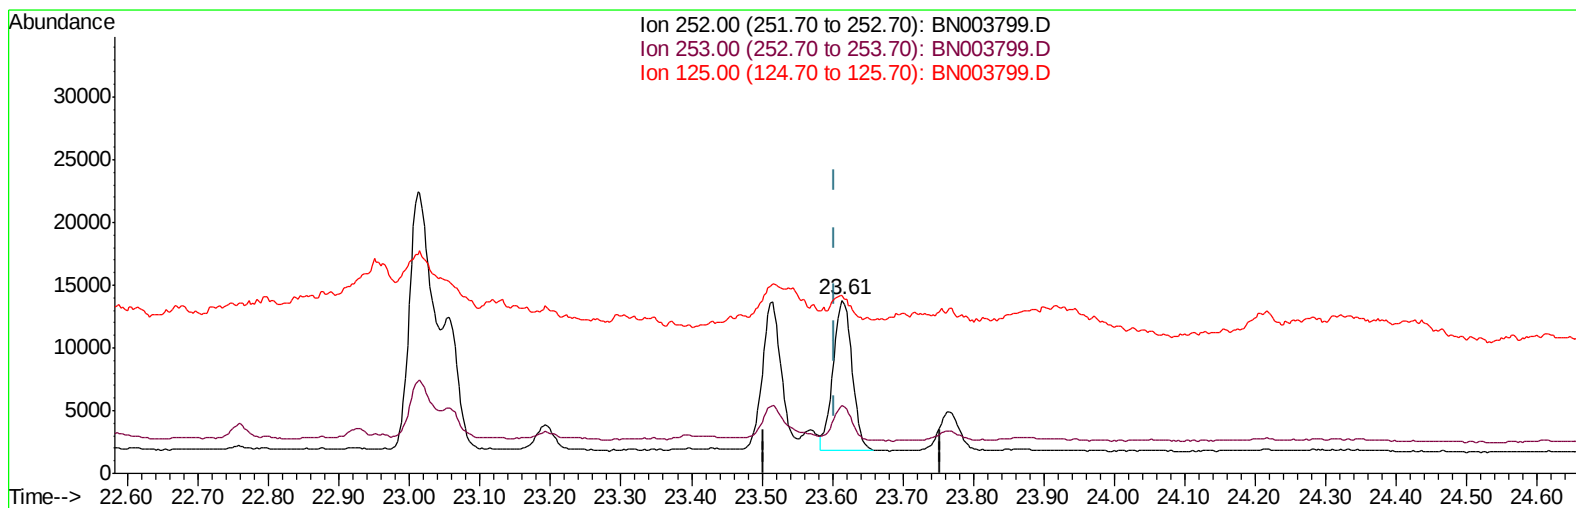

TIC: BN003799.D

(23) Benzo(a)pyrene (C)

23.614min (+0.010) 0.36ng/ul m

response 22439

Ion	Exp%	Act%
252.00	100	100
253.00	23.70	39.10#
125.00	12.80	102.82#
0.00	0.00	0.00