
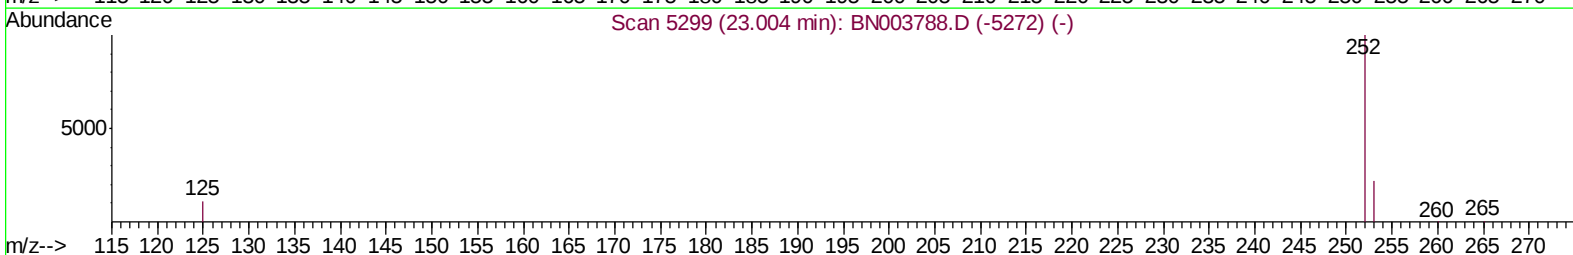
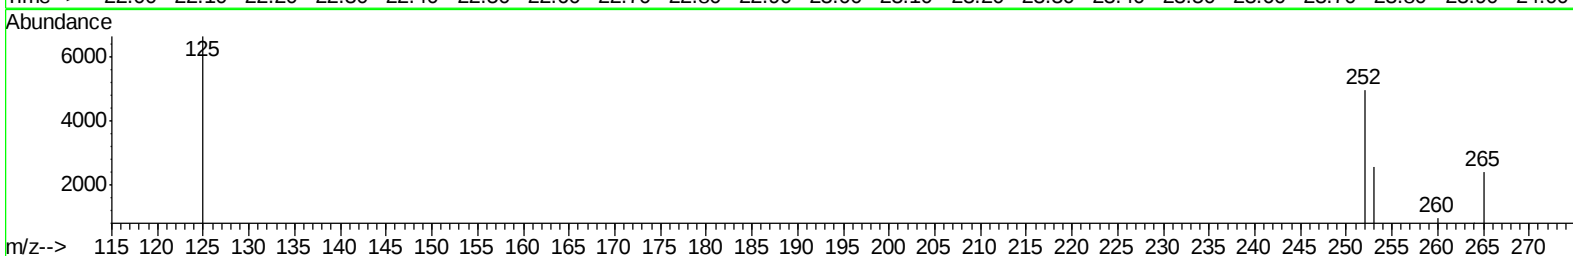


Data File : BN003800.D
Acq On : 11 Dec 2018 04:14
Operator : JU/SJ
Sample : J6077-18DL 5X
Misc :
ALS Vial : 26 Sample Multiplier: 1

Quant Time: Dec 11 08:14:09 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 11 04:22:54 2018
Response via : Initial Calibration

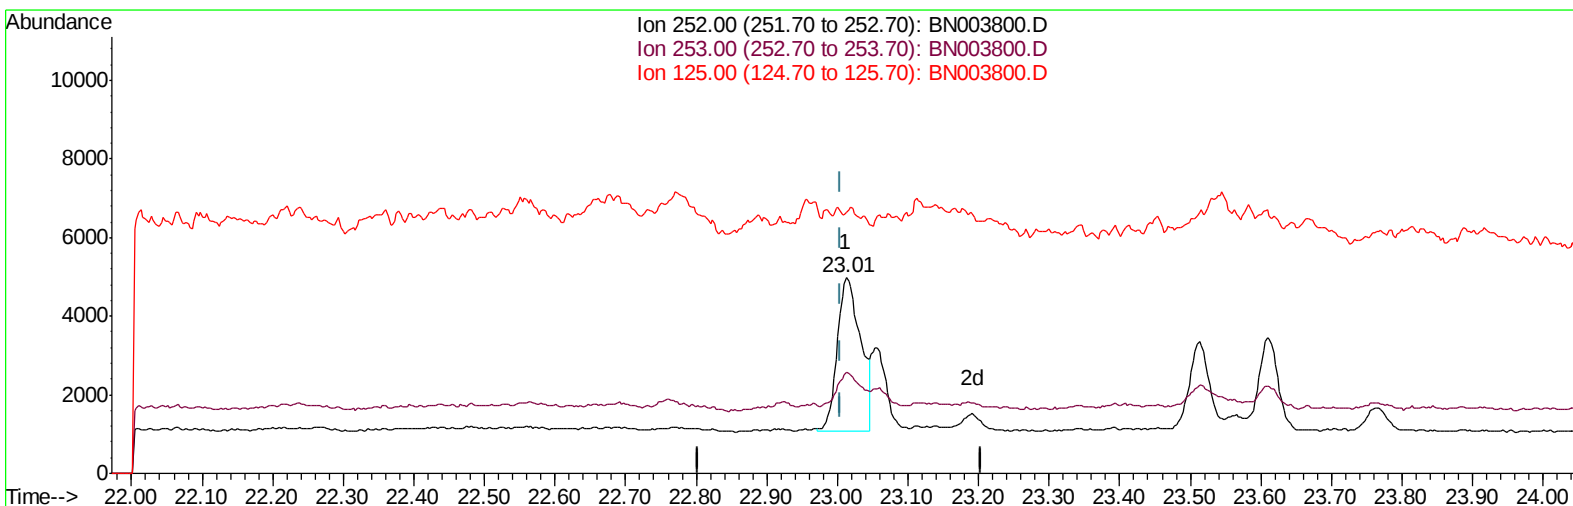

TIC: BN003800.D

(21) Benzo(b)fluoranthene

23.013min (+0.009) 0.14ng/ul m

response 8966

Ion	Exp%	Act%
252.00	100	100
253.00	23.00	51.63#
125.00	11.20	133.71#
0.00	0.00	0.00