
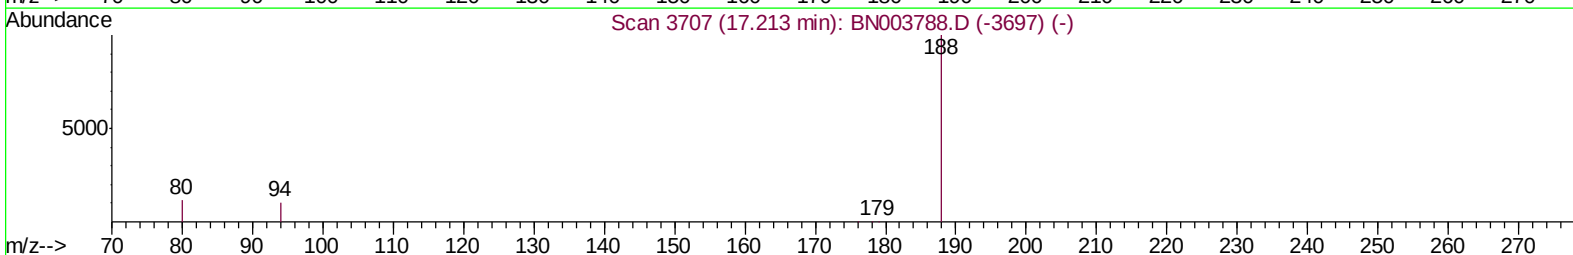
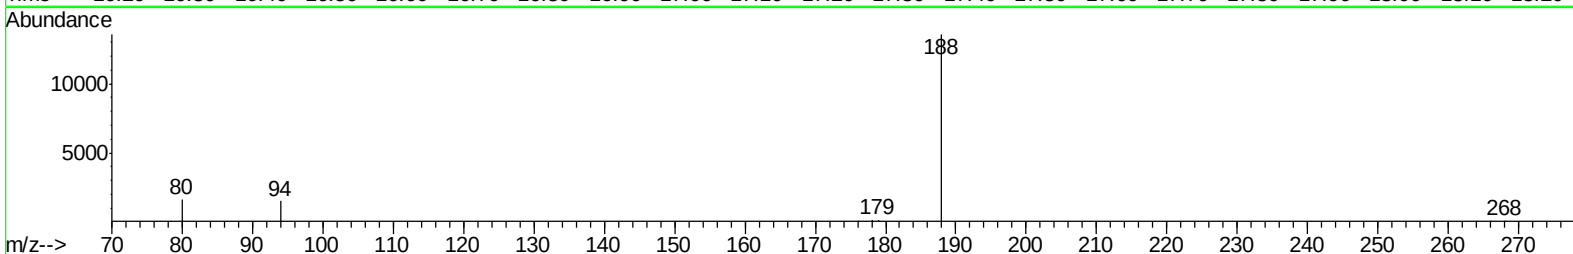


Data File : BN003801.D
Acq On : 11 Dec 2018 04:49
Operator : JU/SJ
Sample : J6077-13
Misc :
ALS Vial : 27 Sample Multiplier: 1

Quant Time: Dec 11 08:14:17 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 11 04:22:54 2018
Response via : Initial Calibration

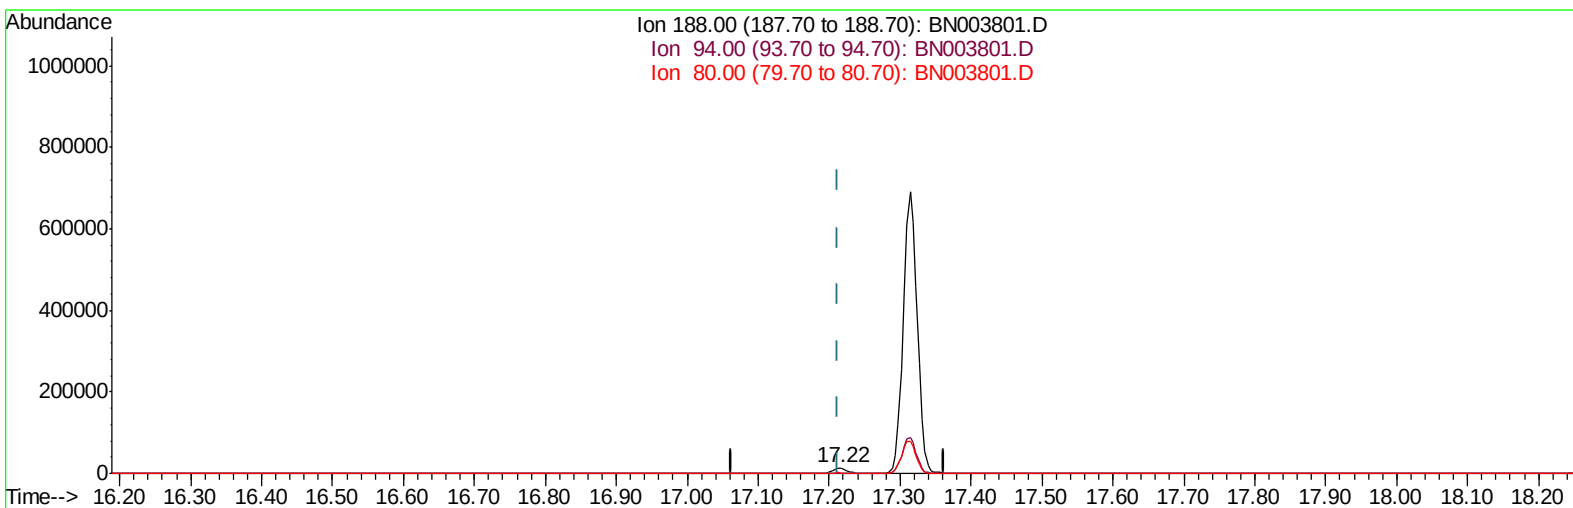

TIC: BN003801.D

(10) Phenanthrene-d10 (I)

17.217min (+0.004) 0.40ng/ul m

response 18793

Ion	Exp%	Act%
188.00	100	100
94.00	10.40	11.20
80.00	11.60	11.96
0.00	0.00	0.00