
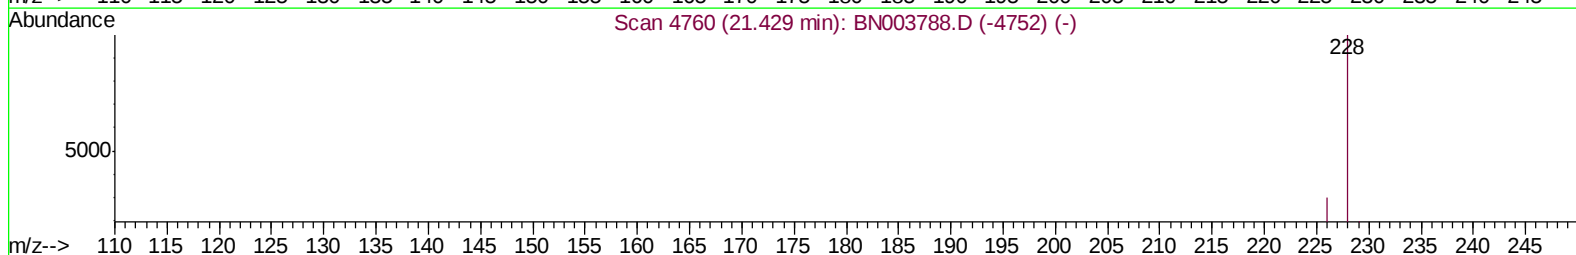
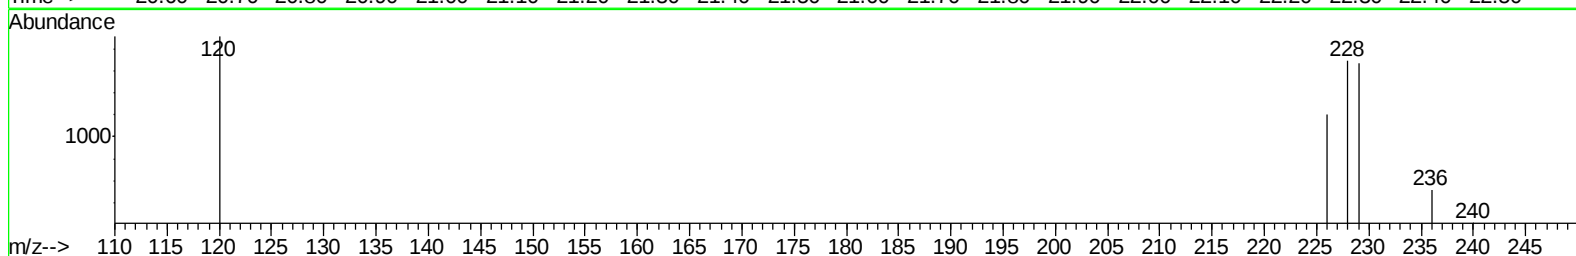


Data File : BN003801.D  
Acq On : 11 Dec 2018 04:49  
Operator : JU/SJ  
Sample : J6077-13  
Misc :  
ALS Vial : 27 Sample Multiplier: 1

Quant Time: Dec 11 08:18:10 2018  
Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_N\METHODS\SOM-EPA-SIM-BN111918.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Tue Dec 11 04:22:54 2018  
Response via : Initial Calibration

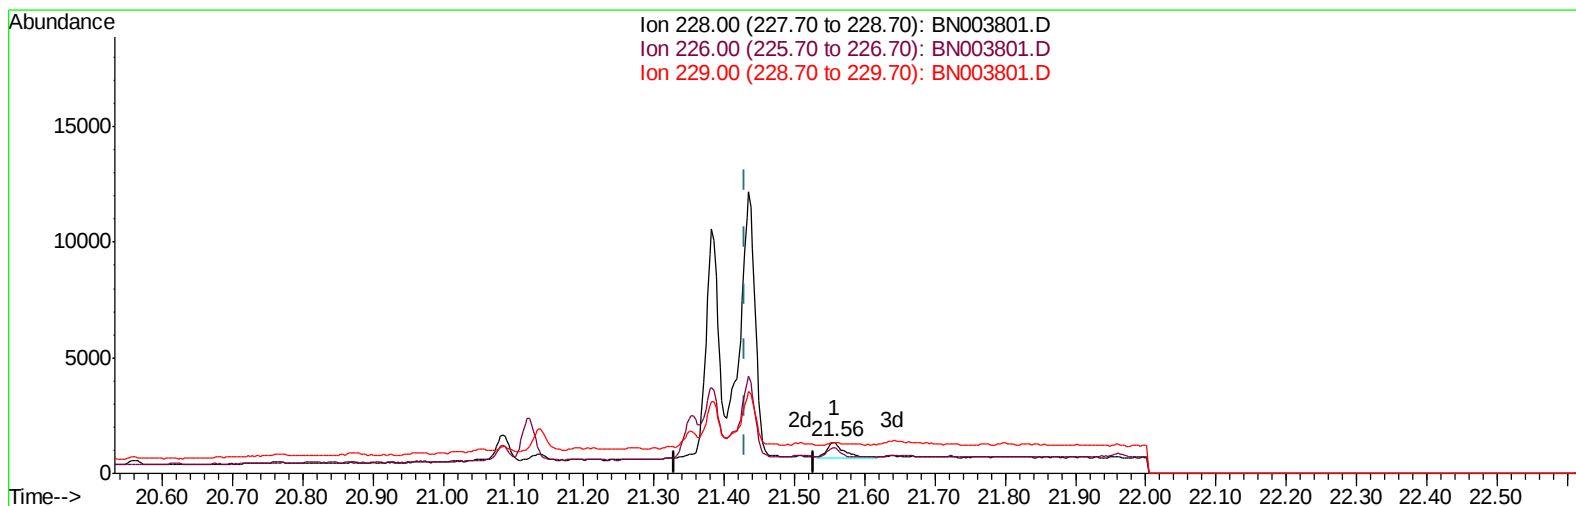

TIC: BN003801.D

(19) Chrysene

21.557min (+0.128) 0.02ng/ul

response 1028

| Ion    | Exp%  | Act%   |
|--------|-------|--------|
| 228.00 | 100   | 100    |
| 226.00 | 30.00 | 81.65# |
| 229.00 | 19.60 | 99.26# |
| 0.00   | 0.00  | 0.00   |