
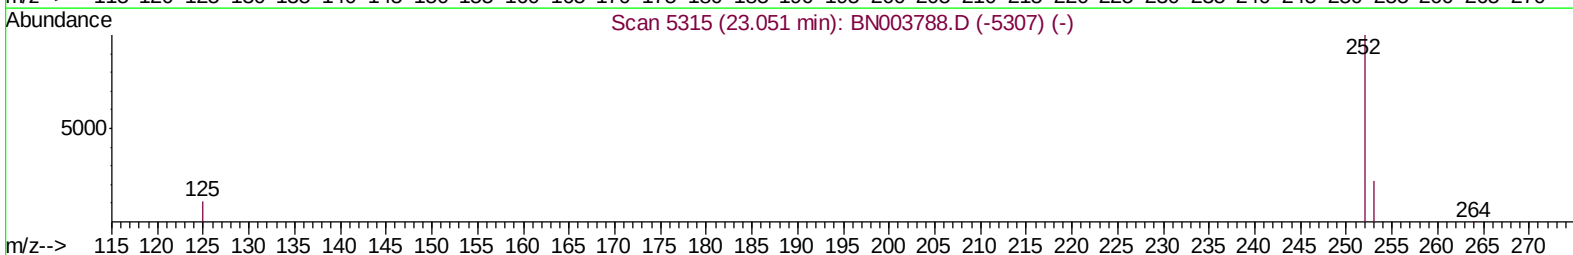
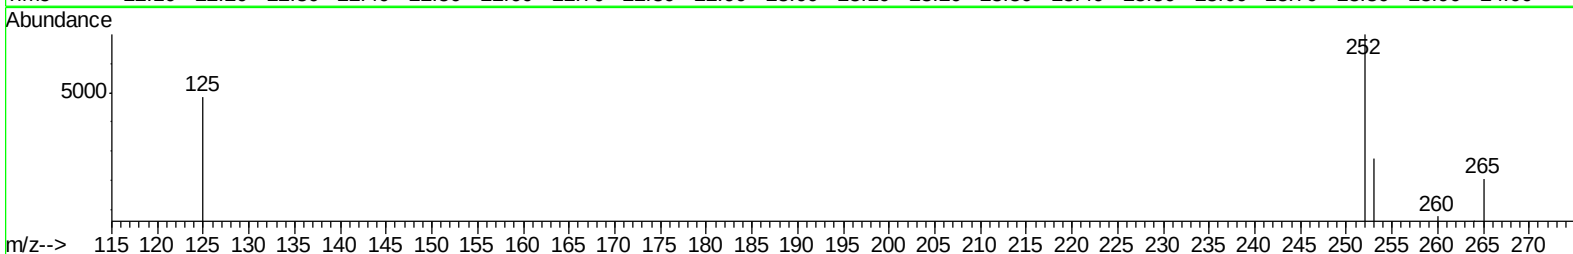


Data File : BN003801.D
Acq On : 11 Dec 2018 04:49
Operator : JU/SJ
Sample : J6077-13
Misc :
ALS Vial : 27 Sample Multiplier: 1

Quant Time: Dec 11 08:18:10 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 11 04:22:54 2018
Response via : Initial Calibration

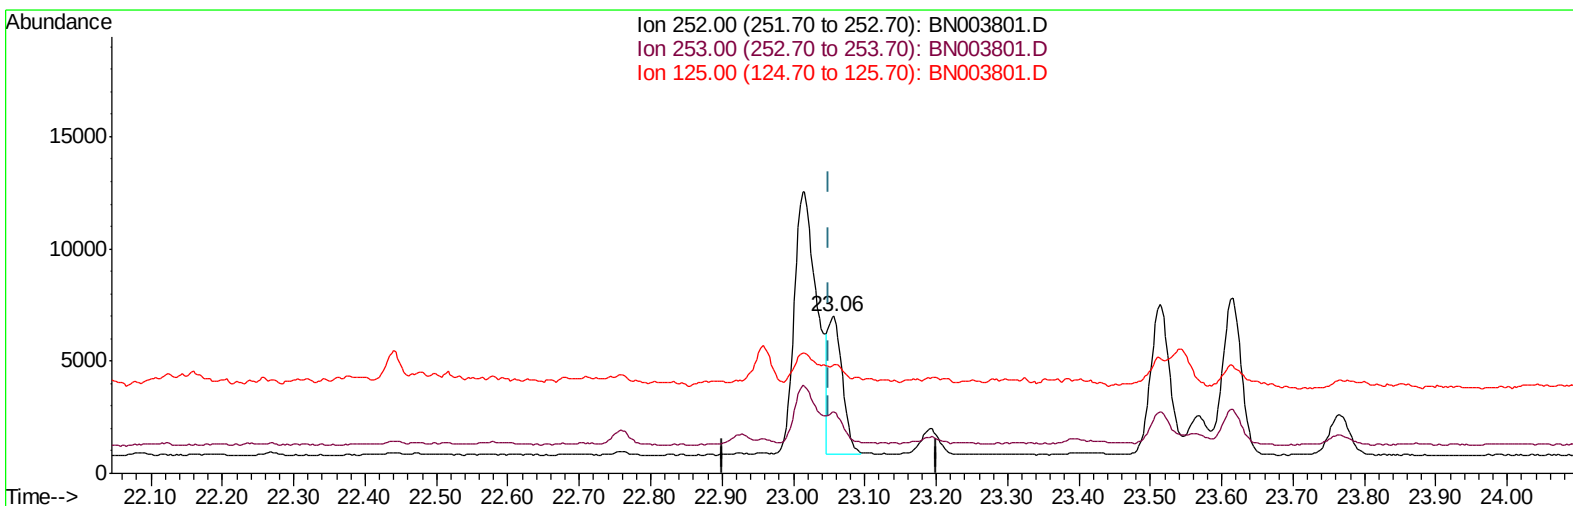

TIC: BN003801.D

(22) Benzo(k)fluoranthene

23.057min (+0.006) 0.14ng/ul m

response 8828

Ion	Exp%	Act%
252.00	100	100
253.00	23.10	39.16#
125.00	11.30	69.42#
0.00	0.00	0.00