
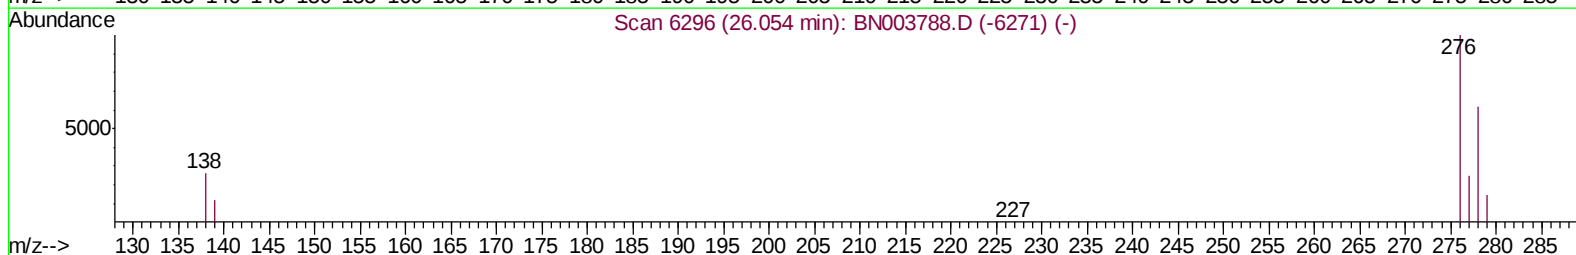
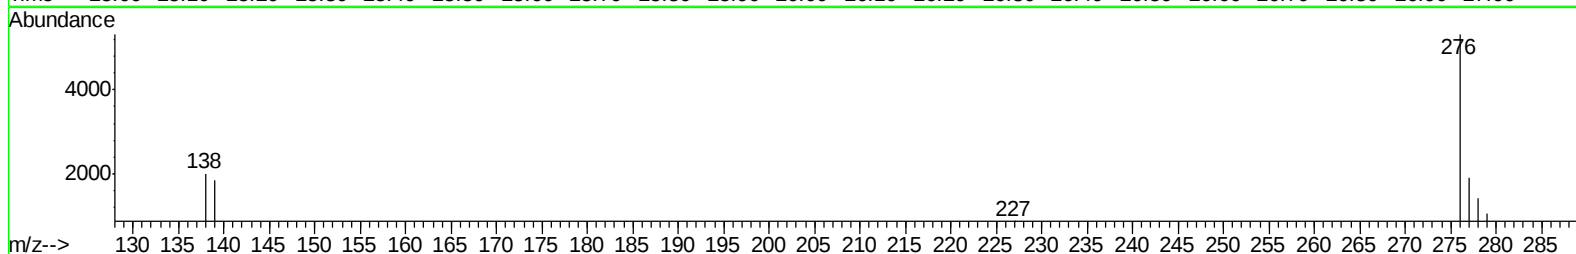


Data File : BN003801.D
Acq On : 11 Dec 2018 04:49
Operator : JU/SJ
Sample : J6077-13
Misc :
ALS Vial : 27 Sample Multiplier: 1

Quant Time: Dec 11 08:18:10 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 11 04:22:54 2018
Response via : Initial Calibration

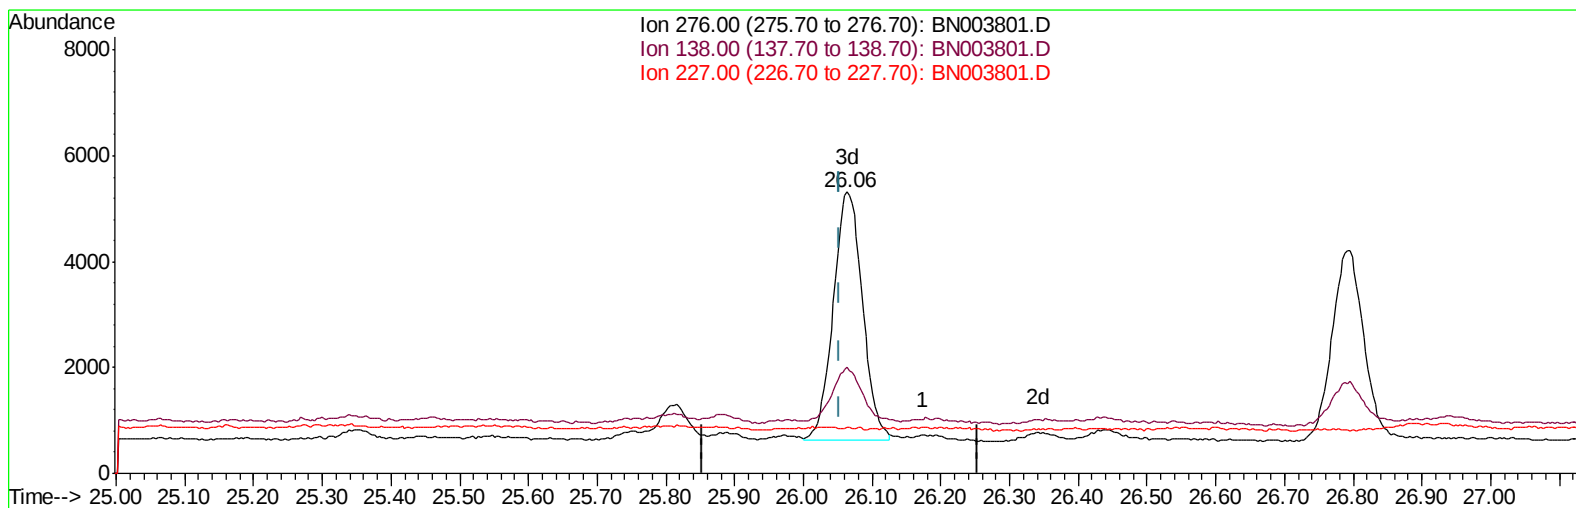

TIC: BN003801.D

(24) Indeno(1,2,3-cd)pyrene

26.064min (+0.010) 0.22ng/ul m

response 13777

Ion	Exp%	Act%
276.00	100	100
138.00	25.40	0.00#
227.00	0.20	0.19
0.00	0.00	0.00