
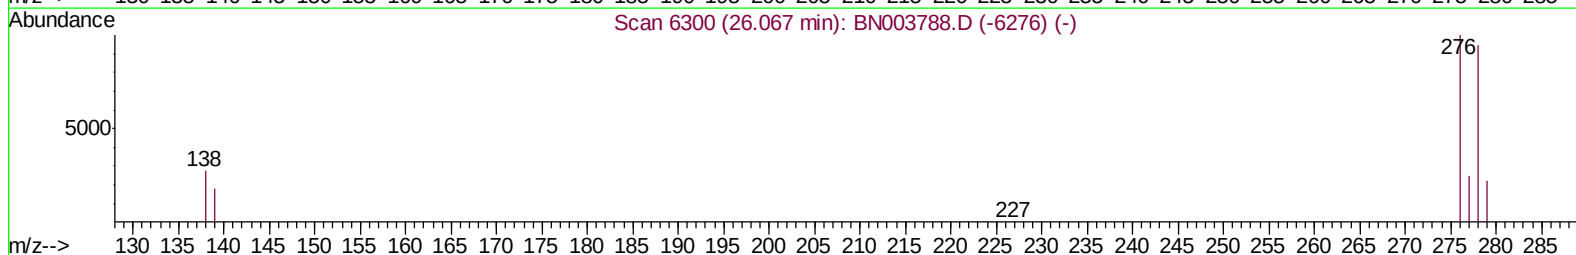
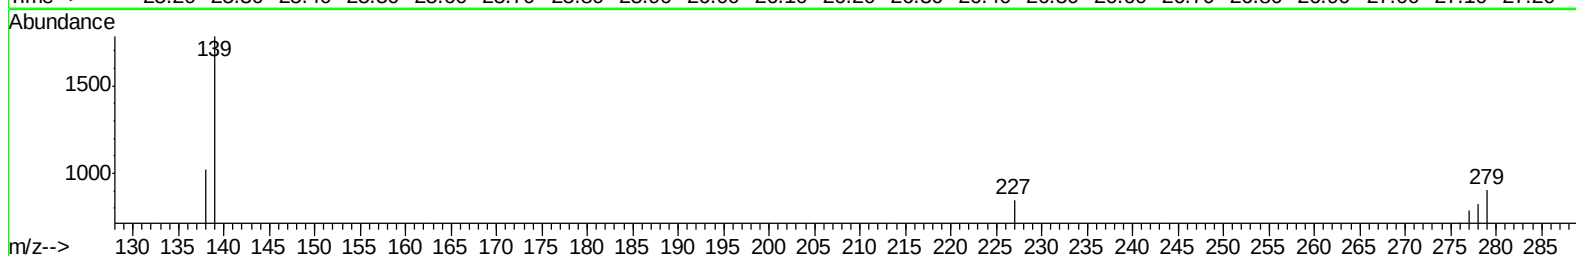


Data File : BN003801.D  
Acq On : 11 Dec 2018 04:49  
Operator : JU/SJ  
Sample : J6077-13  
Misc :  
ALS Vial : 27 Sample Multiplier: 1

Quant Time: Dec 11 08:18:10 2018  
Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_N\METHODS\SOM-EPA-SIM-BN111918.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Tue Dec 11 04:22:54 2018  
Response via : Initial Calibration

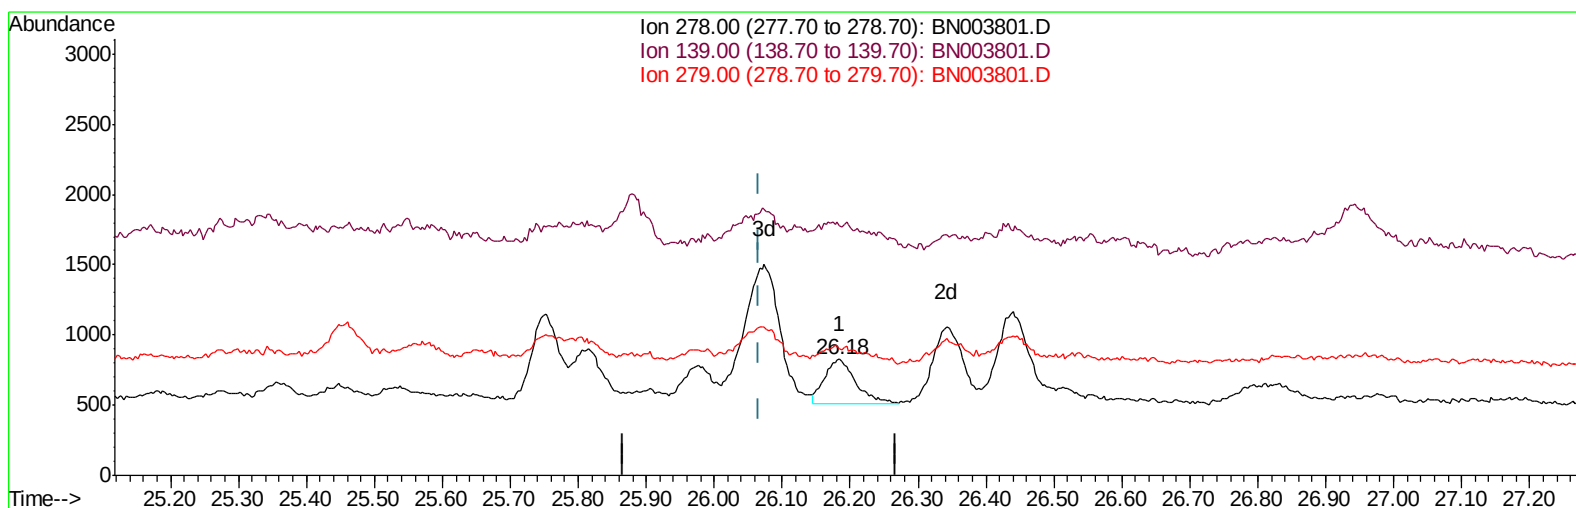

TIC: BN003801.D

(25) Dibenzo(a,h)anthracene

26.184min (+0.117) 0.02ng/ul

response 995

| Ion    | Exp%  | Act%    |
|--------|-------|---------|
| 278.00 | 100   | 100     |
| 139.00 | 17.80 | 215.36# |
| 279.00 | 24.70 | 109.55# |
| 0.00   | 0.00  | 0.00    |