
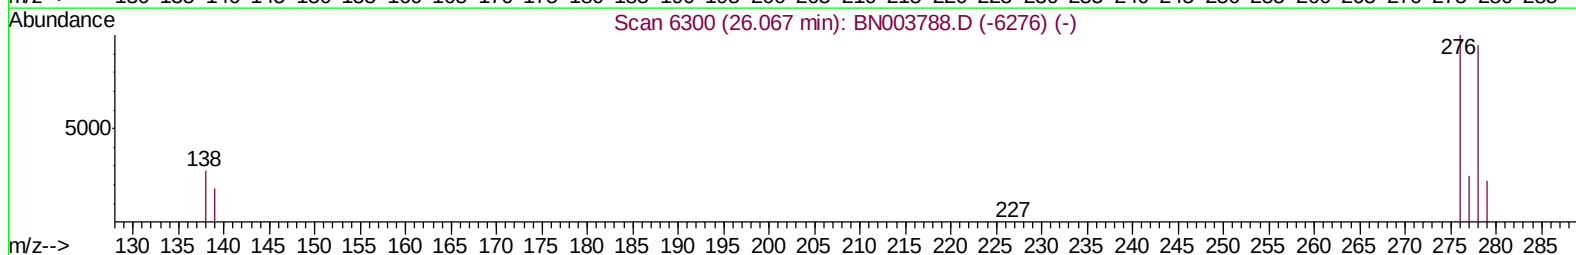
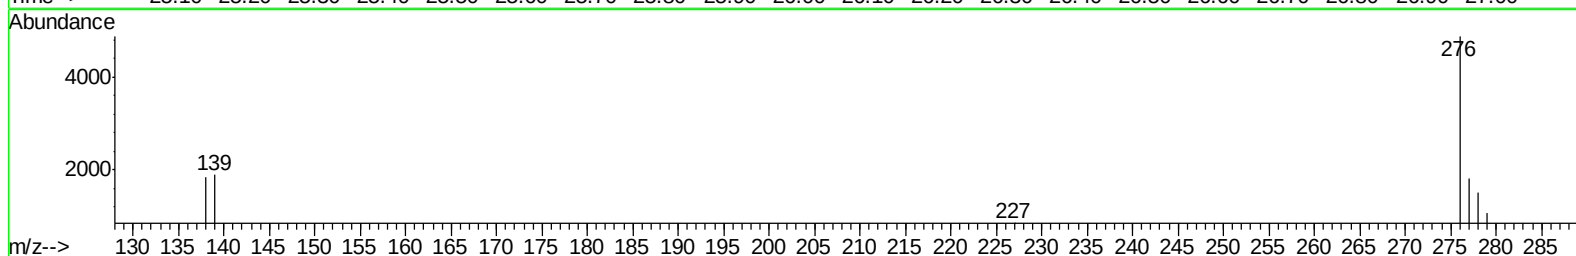


Data File : BN003801.D
Acq On : 11 Dec 2018 04:49
Operator : JU/SJ
Sample : J6077-13
Misc :
ALS Vial : 27 Sample Multiplier: 1

Quant Time: Dec 11 08:18:10 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 11 04:22:54 2018
Response via : Initial Calibration

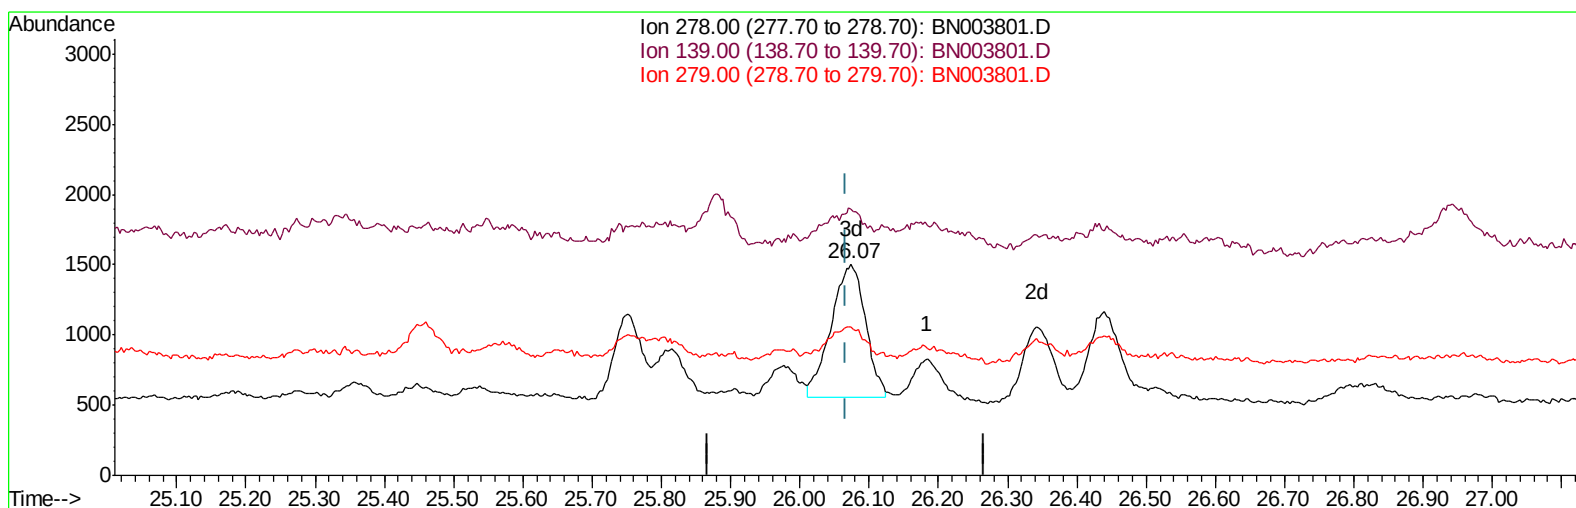

TIC: BN003801.D

(25) Dibenzo(a,h)anthracene

26.074min (+0.007) 0.06ng/ul m

response 3274

Ion	Exp%	Act%
278.00	100	100
139.00	17.80	125.71#
279.00	24.70	70.43#
0.00	0.00	0.00