
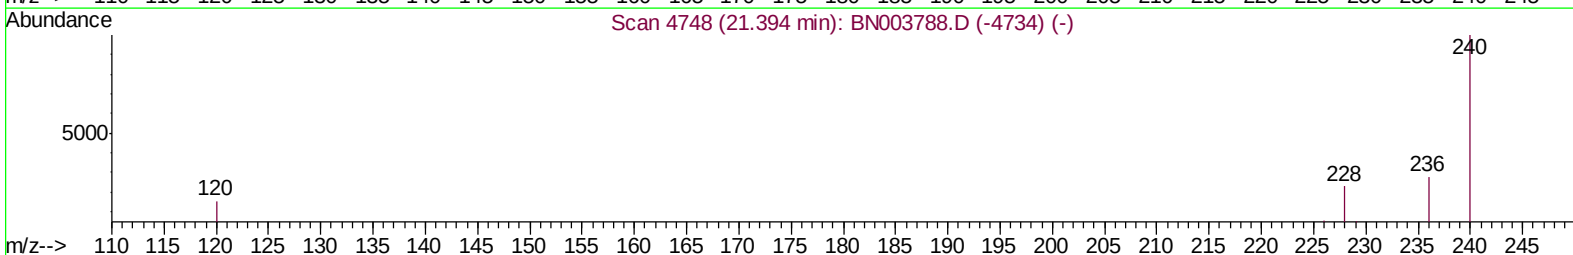
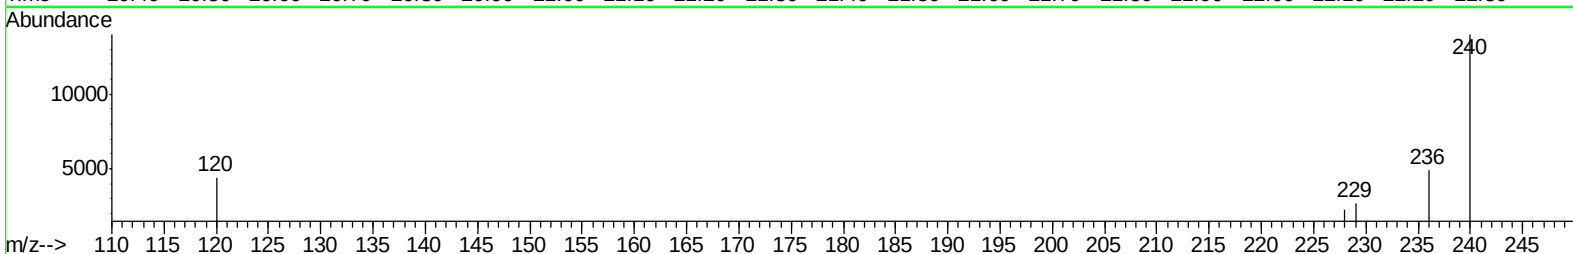


Data File : BN003802.D
Acq On : 11 Dec 2018 05:24
Operator : JU/SJ
Sample : J6077-19
Misc :
ALS Vial : 28 Sample Multiplier: 1

Quant Time: Dec 11 08:22:12 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 11 04:22:54 2018
Response via : Initial Calibration

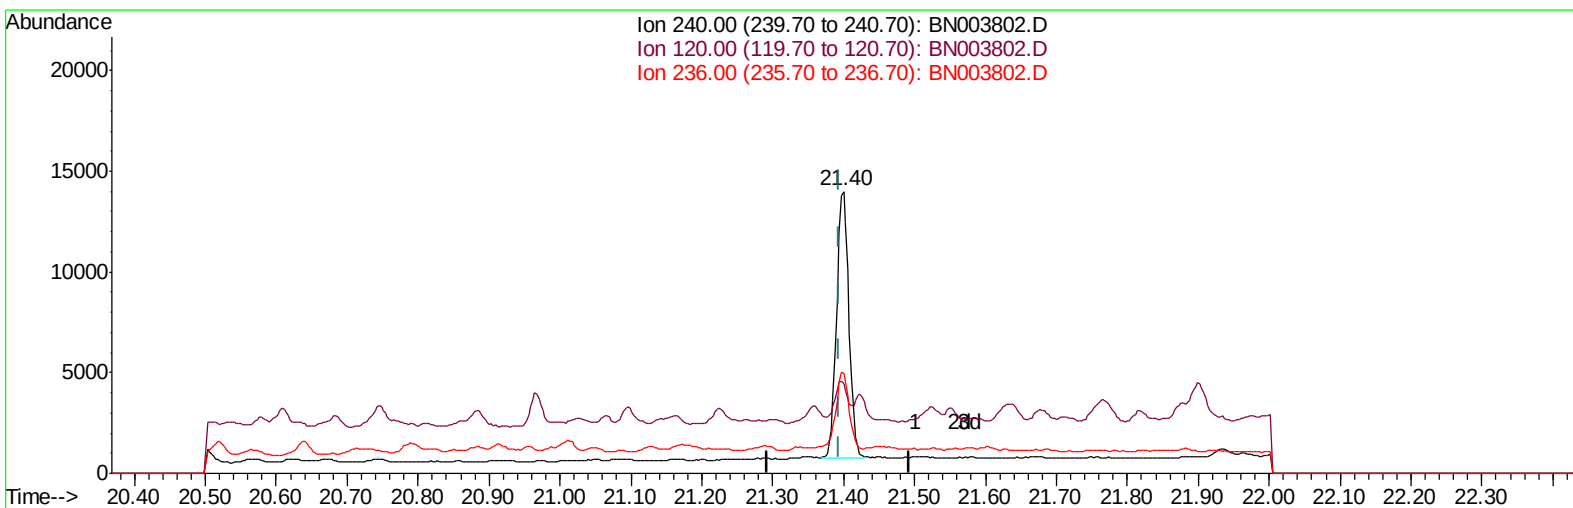

TIC: BN003802.D

(16) Chrysene-d12 (I)

21.400min (+0.006) 0.40ng/ul m

response 15967

Ion	Exp%	Act%
240.00	100	100
120.00	14.00	31.83#
236.00	27.60	35.46#
0.00	0.00	0.00