
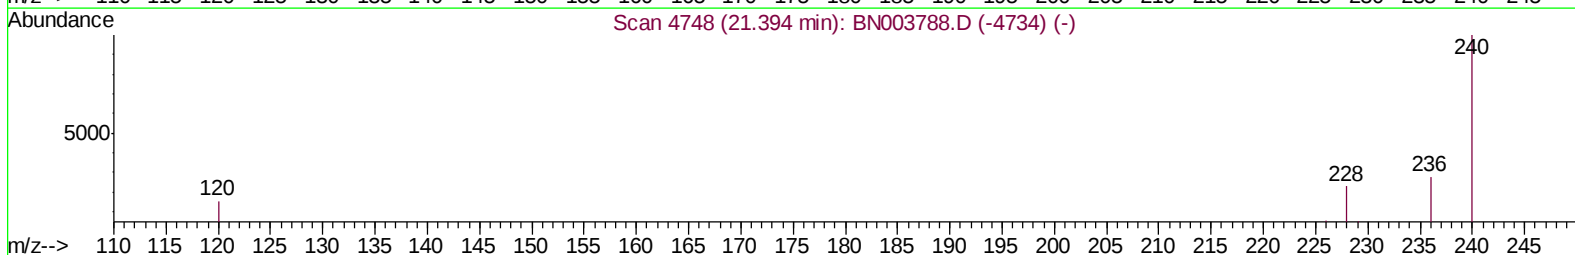
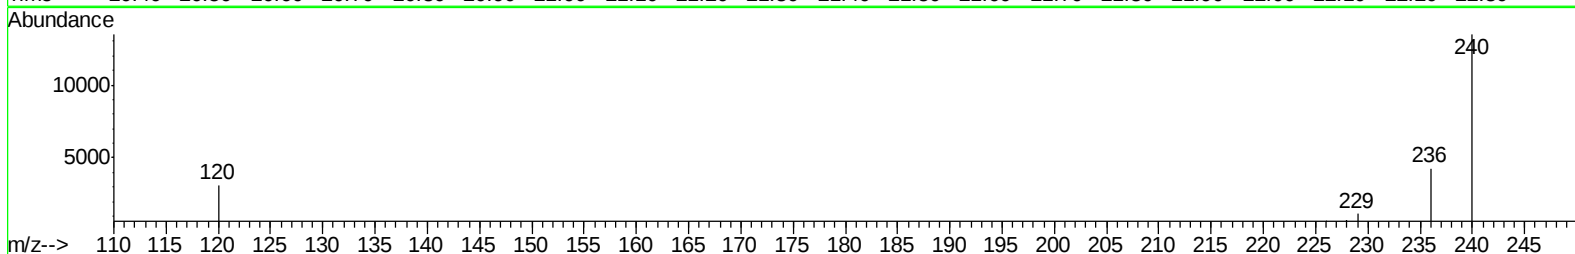


Data File : BN003803.D
Acq On : 11 Dec 2018 05:59
Operator : JU/SJ
Sample : J6077-17
Misc :
ALS Vial : 29 Sample Multiplier: 1

Quant Time: Dec 11 08:26:11 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 11 04:22:54 2018
Response via : Initial Calibration

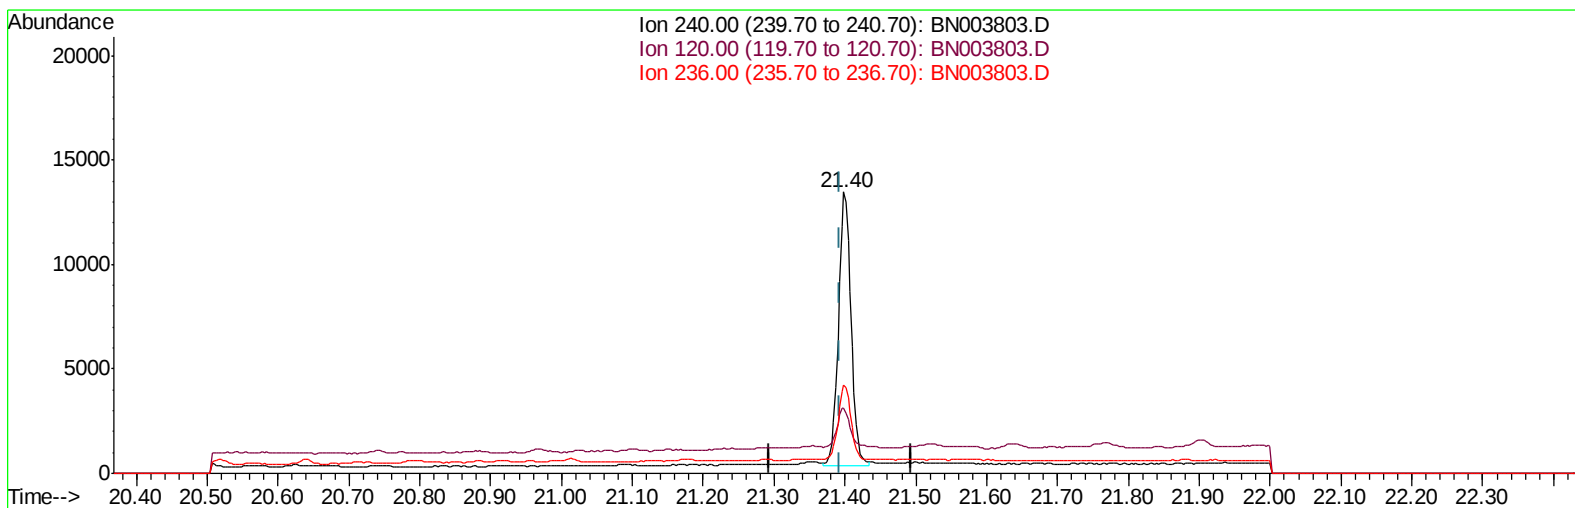

TIC: BN003803.D

(16) Chrysene-d12 (I)

21.399min (+0.005) 0.40ng/ul m

response 16115

Ion	Exp%	Act%
240.00	100	100
120.00	14.00	23.37#
236.00	27.60	31.60
0.00	0.00	0.00