

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN121018\
Quantitation Report (Not Reviewed)

Data File : BN003780.D
Acq On : 10 Dec 2018 15:57
Operator : JU/SJ
Sample : PB115355BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK55

Quant Time: Dec 11 03:45:19 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 11 03:42:06 2018
Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.84	152	4769	0.40	ng/ul	0.00
2) Naphthalene-d8	10.63	136	19627	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.47	164	10824	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.31	188	1613532	0.40	ng/ul	0.10
16) Chrysene-d12	0.00	240	0	0.00	ng/ul	-21.40
20) Perylene-d12	23.71	264	18994	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.22	152	9668	0.32	ng/ul	0.00
14) Fluoranthene-d10	0.00	212	0	0.00	ng/ul	
Target Compounds						
23) Benzo(a)pyrene	23.57	252	5593	0.082	ng/ul#	Qvalue 65


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data File : BN003780.D
Acq On : 10 Dec 2018 15:57
Operator : JU/SJ
Sample : PB115355BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK55

Quant Time: Dec 11 03:45:19 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 11 03:42:06 2018
Response via : Initial Calibration

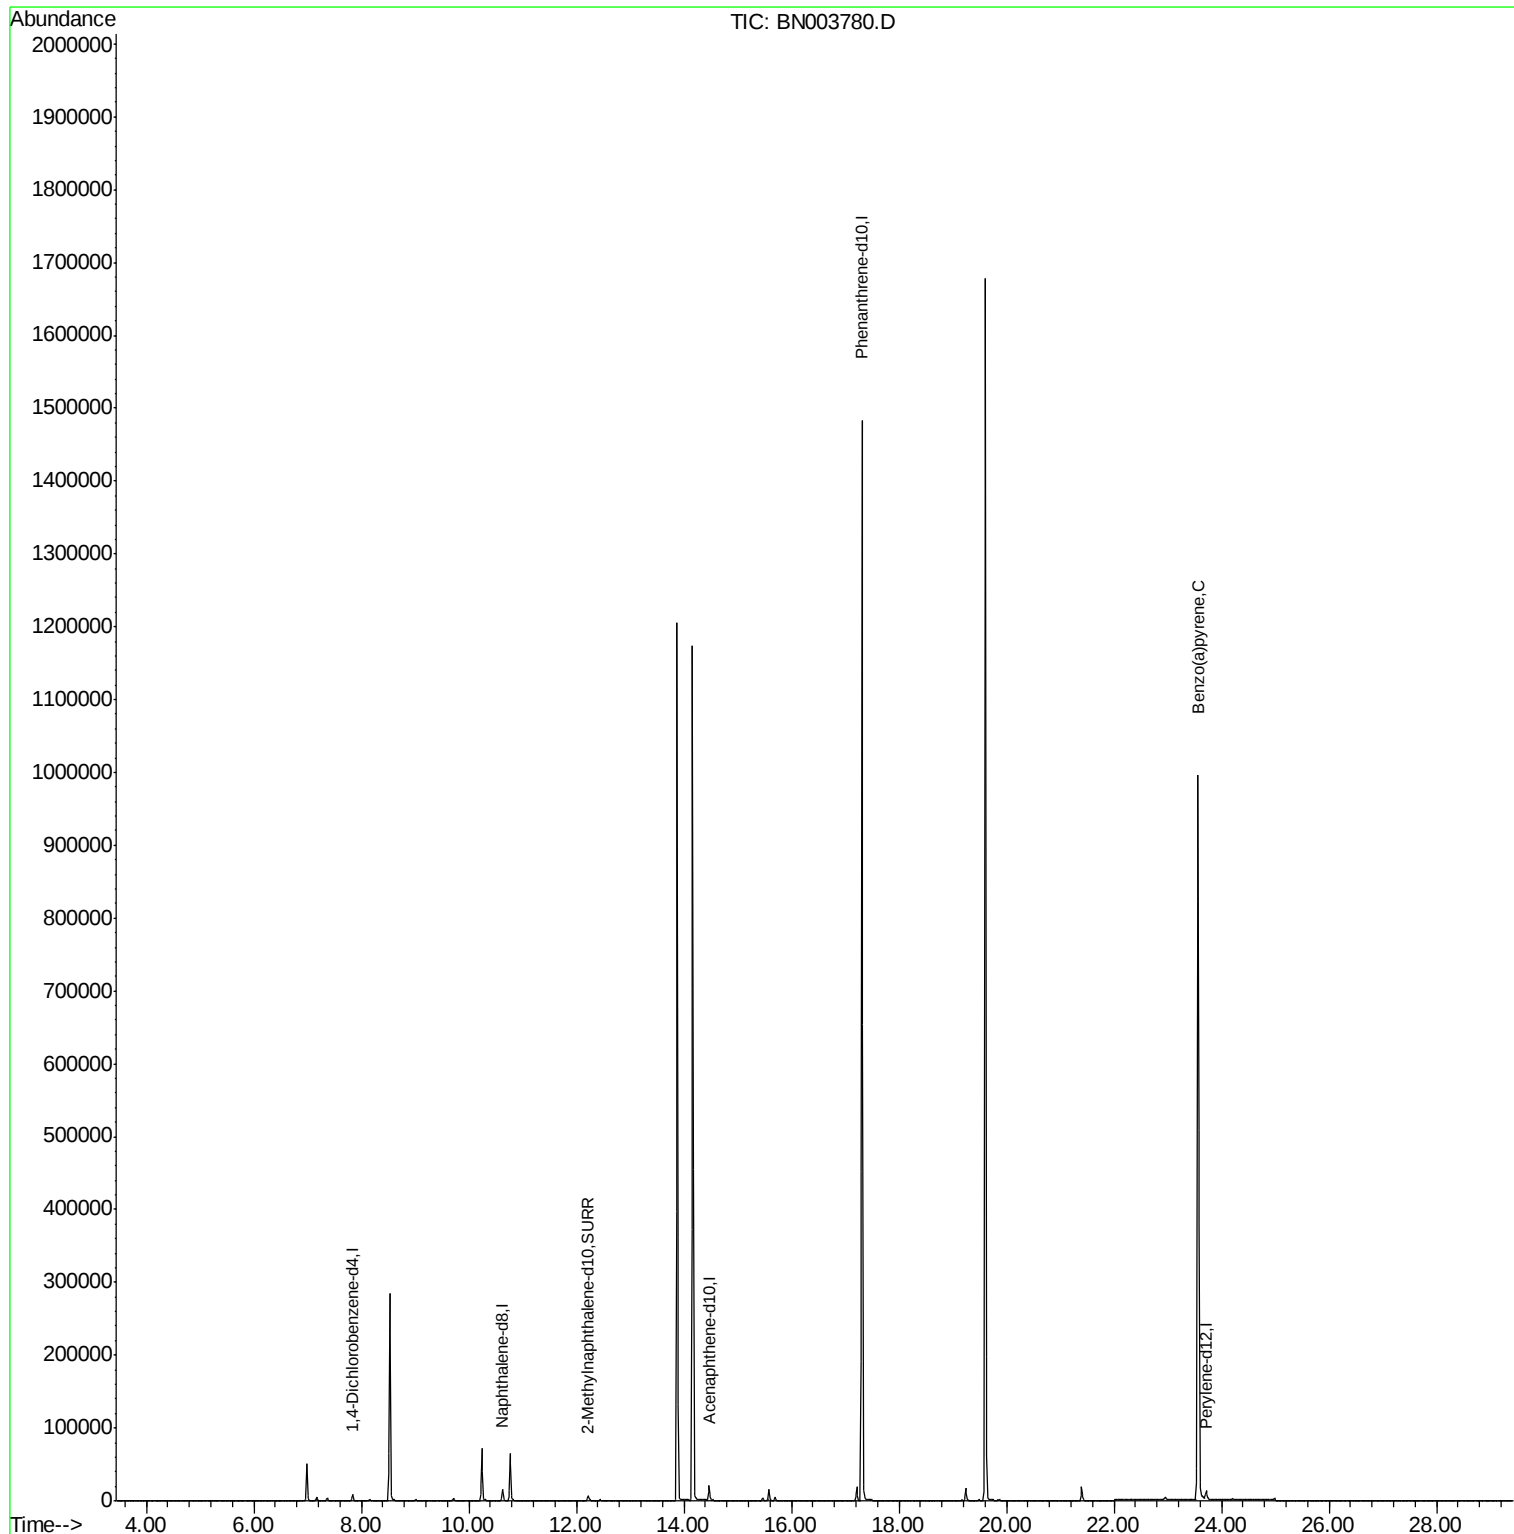

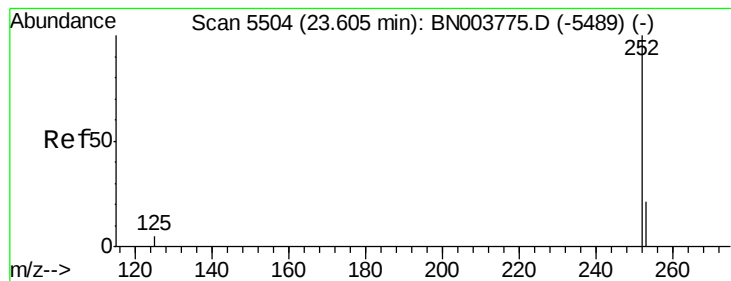

#23

Benzo(a)pyrene

Concen: 0.082 ng/ul

RT: 23.57 min Scan# 5491

Delta R.T. -0.04 min

Lab File: BN003780.D


Acq: 10 Dec 2018 15:57

Instrument :

BNA_N

ClientSampleId :

SBLK55

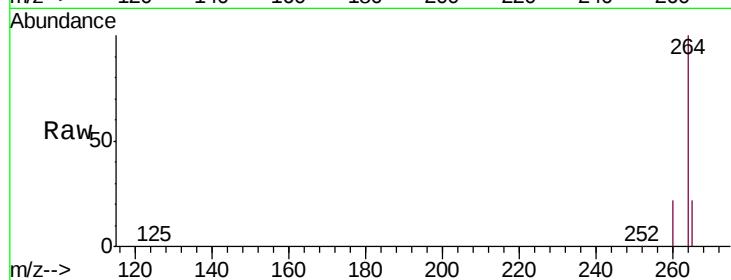

Tgt Ion:	252	Resp:	5593
Ion	Ratio	Lower	Upper
252	100		
253	36.9	19.0	28.4#
125	32.6	10.2	15.4#

