

Data Path : Z:\SVOASRV\HPCHEM1\BNA_N\DATA\BN121018\
Quantitation Report (Not Reviewed)

Data File : BN003782.D
Acq On : 10 Dec 2018 17:08
Operator : JU/SJ
Sample : J6155-16
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A4118

Quant Time: Dec 11 03:45:30 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 11 03:42:06 2018
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.84	152	5294	0.40	ng/ul	0.00
2) Naphthalene-d8	10.63	136	21447	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.47	164	11309	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.21	188	24040	0.40	ng/ul	0.00
16) Chrysene-d12	21.40	240	18342	0.40	ng/ul	0.00
20) Perylene-d12	23.71	264	17707	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.22	152	3534	0.11	ng/ul	0.00
14) Fluoranthene-d10	19.24	212	7457	0.11	ng/ul	0.00
Target Compounds						
23) Benzo(a)pyrene	23.57	252	2004	0.032	ng/ul#	Qvalue 19

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data File : BN003782.D

Acq On : 10 Dec 2018 17:08

Operator : JU/SJ

Sample : J6155-16

Misc :

ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
A4118


Quant Time: Dec 11 03:45:30 2018


Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Tue Dec 11 03:42:06 2018

Response via : Initial Calibration

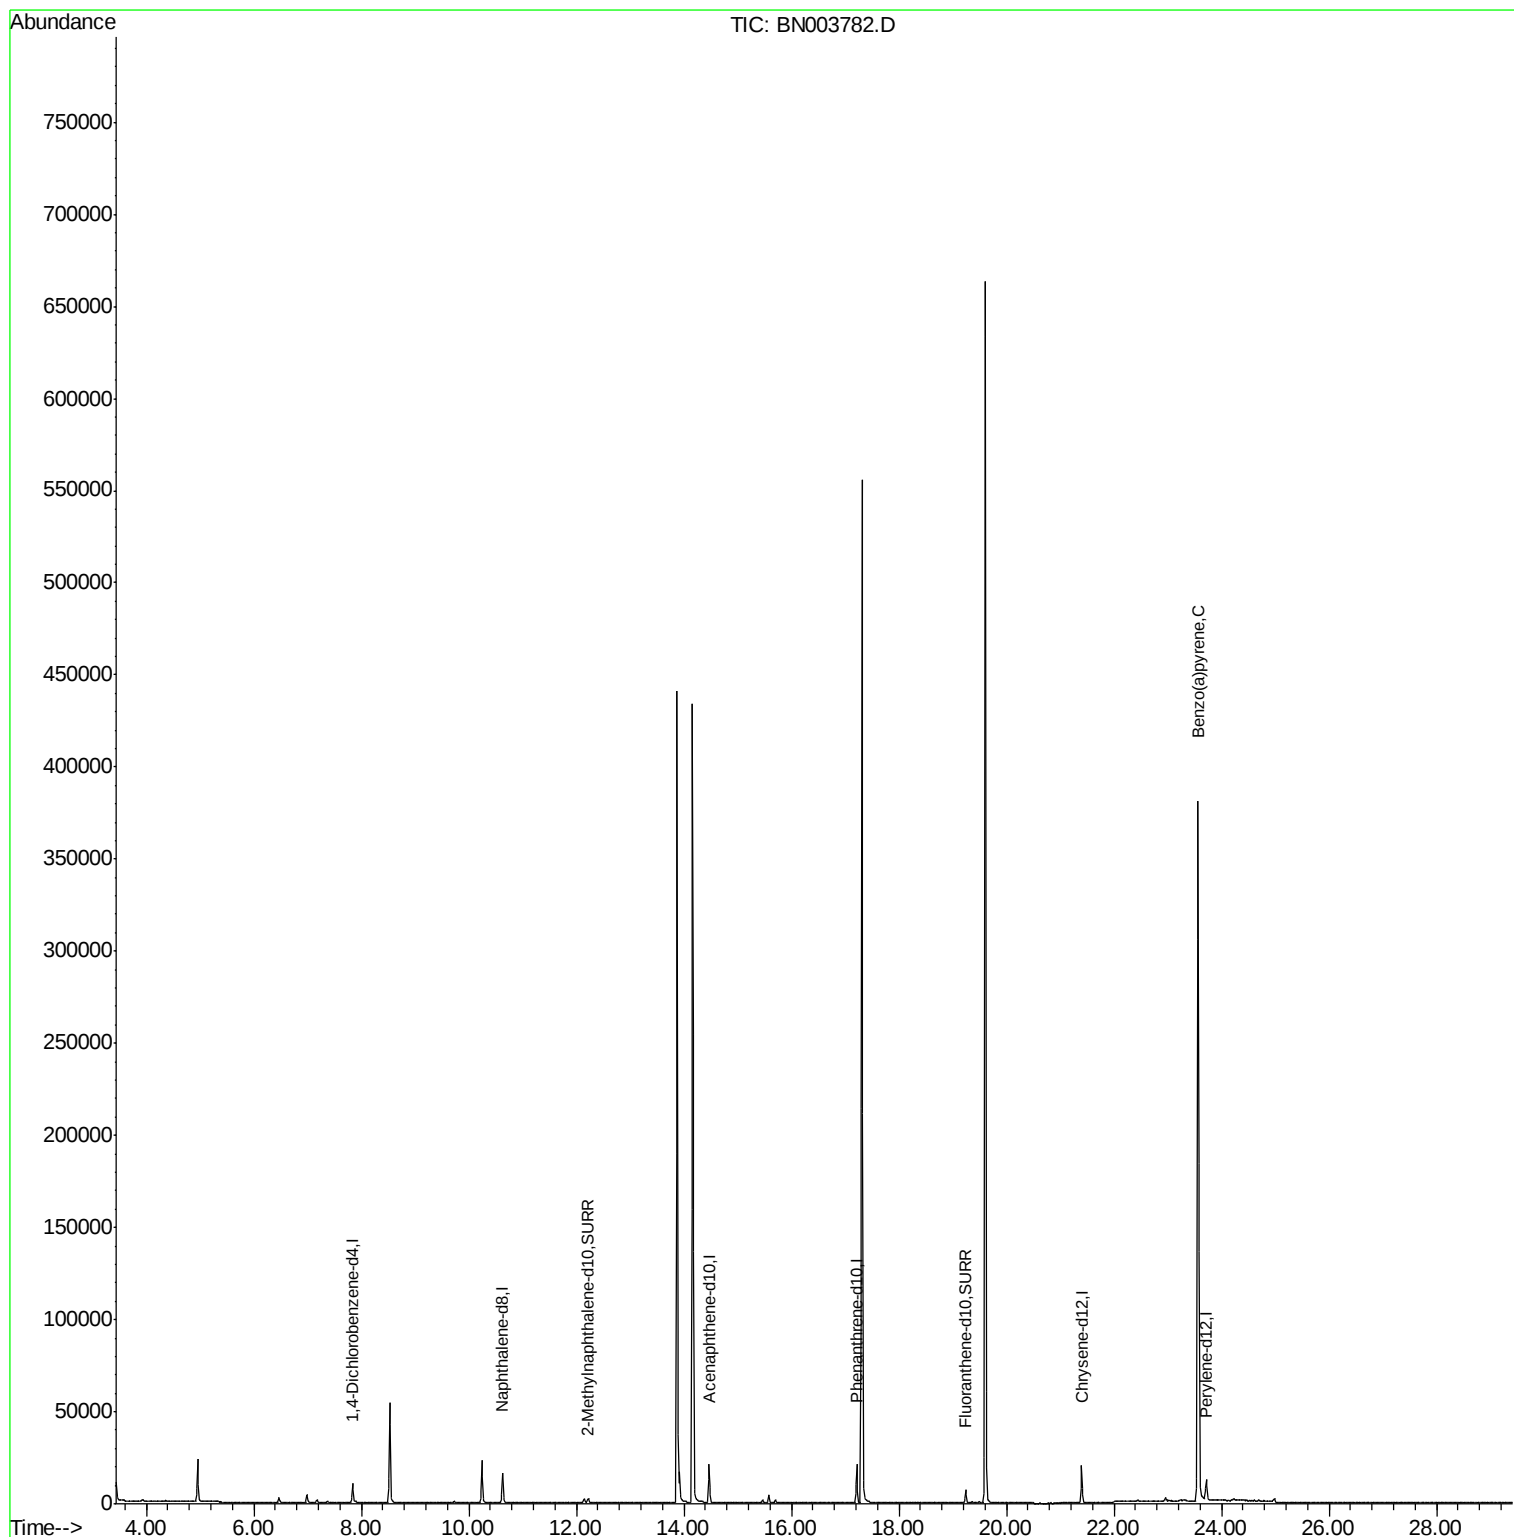

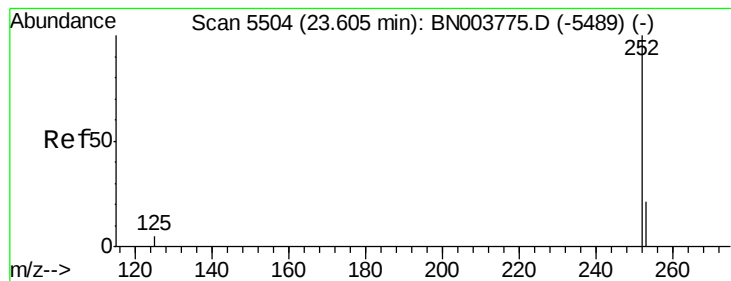

#23

Benzo(a)pyrene

Concen: 0.032 ng/ul

RT: 23.57 min Scan# 5491

Delta R.T. -0.04 min

Lab File: BN003782.D


Acq: 10 Dec 2018 17:08

Instrument :

BNA_N

ClientSampleId :

A4118

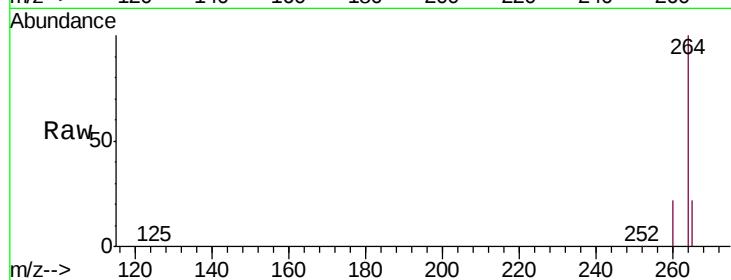

Tgt Ion: 252 Resp: 2004

Ion Ratio Lower Upper

252 100

253 56.4 19.0 28.4#

125 55.8 10.2 15.4#

