

Data File : BN003798.D
Acq On : 11 Dec 2018 03:04
Operator : JU/SJ
Sample : J6077-16DL 5X
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
F9Y32DL

Quant Time: Dec 11 04:27:50 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 11 04:22:54 2018
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.84	152	5720	0.40	ng/ul	0.00
2) Naphthalene-d8	10.63	136	22636	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.48	164	15637	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.22	188	20401	0.40	ng/ul	0.00
16) Chrysene-d12	21.40	240	14755	0.40	ng/ul	0.00
20) Perylene-d12	23.72	264	16610	0.40	ng/ul	0.02

System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.19	152	6783	0.20	ng/ul	-0.02
14) Fluoranthene-d10	19.24	212	3259	0.05	ng/ul	0.00


Target Compounds				Qvalue		
3) Naphthalene	10.68	128	529957	8.335	ng/ul	99
5) 2-Methylnaphthalene	12.30	142	124794	2.811	ng/ul	100
7) Acenaphthylene	14.20	152	13217	0.188	ng/ul#	1
8) Acenaphthene	14.54	153	30924	0.501	ng/ul#	89
9) Fluorene	15.53	166	34369	0.478	ng/ul#	79
11) Pentachlorophenol	16.87	266	578	0.157	ng/ul#	25
12) Phenanthrene	17.26	178	83532	1.248	ng/ul#	79
13) Anthracene	17.36	178	13968	0.254	ng/ul#	38
15) Fluoranthene	19.28	202	33047	0.418	ng/ul	82
17) Pyrene	19.64	202	65323	1.234	ng/ul#	90
18) Benzo(a)anthracene	21.39	228	5876	0.126	ng/ul#	1
19) Chrysene	21.42	228	42765	0.802	ng/ul#	43
21) Benzo(b)fluoranthene	23.02	252	10130	0.147	ng/ul#	1
23) Benzo(a)pyrene	23.62	252	4357	0.073	ng/ul#	1
24) Indeno(1,2,3-cd)pyrene	26.08	276	2469	0.036	ng/ul#	50
26) Benzo(g,h,i)perylene	26.81	276	7299	0.123	ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data File : BN003798.D
Acq On : 11 Dec 2018 03:04
Operator : JU/SJ
Sample : J6077-16DL 5X
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
F9Y32DL

Quant Time: Dec 11 04:27:50 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\SOM-EPA-SIM-BN11918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 11 04:22:54 2018
Response via : Initial Calibration

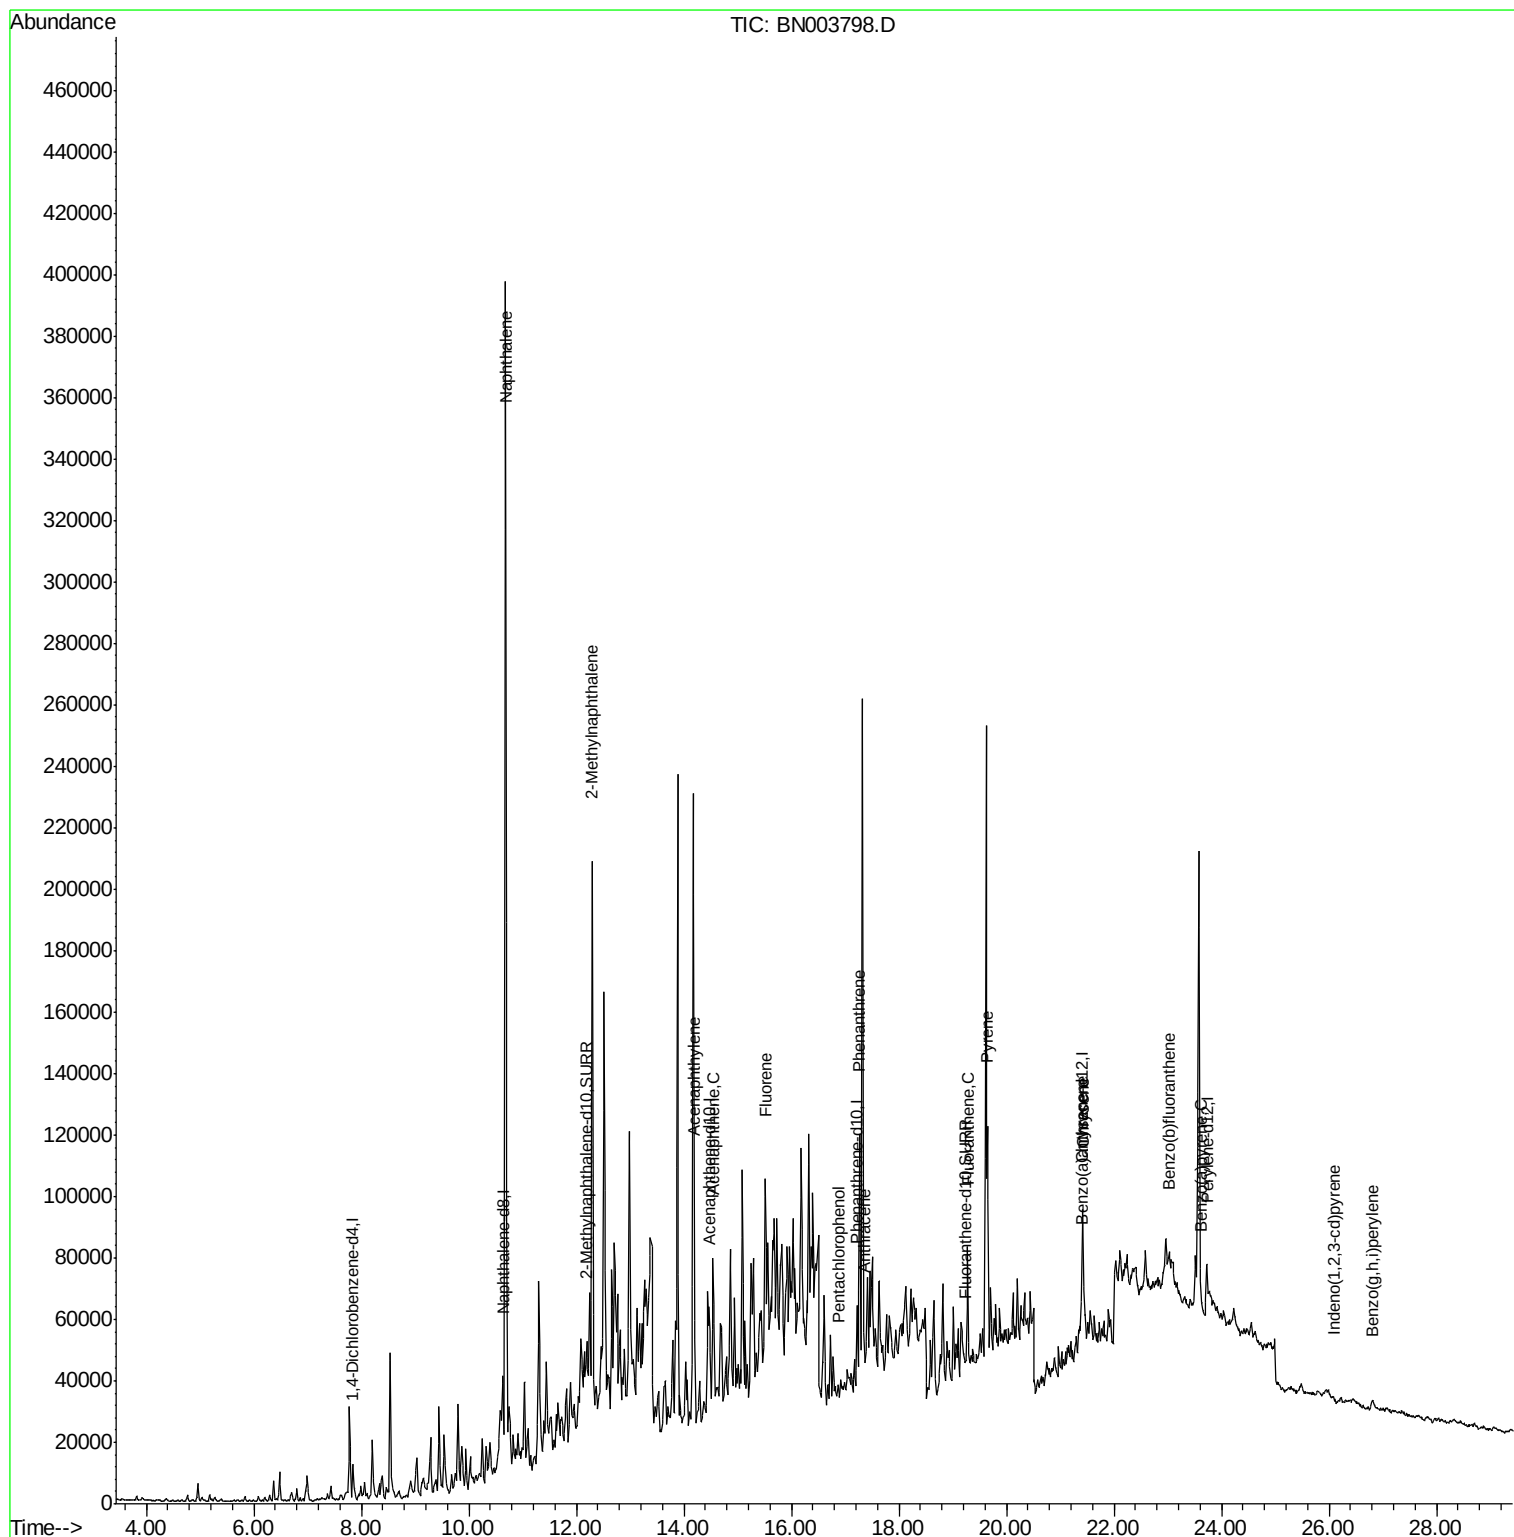

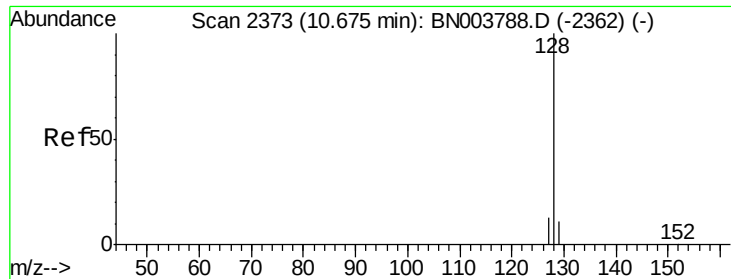

#3

Naphthalene

Concen: 8.335 ng/ul

RT: 10.68 min Scan# 2374

Delta R.T. 0.01 min

Lab File: BN003798.D

Acq: 11 Dec 2018 03:04

Instrument :

BNA_N

ClientSampleId :

F9Y32DL


Tgt Ion:128 Resp: 529957

Ion Ratio Lower Upper

128 100

129 11.6 9.0 13.6




127 13.3 10.5 15.7

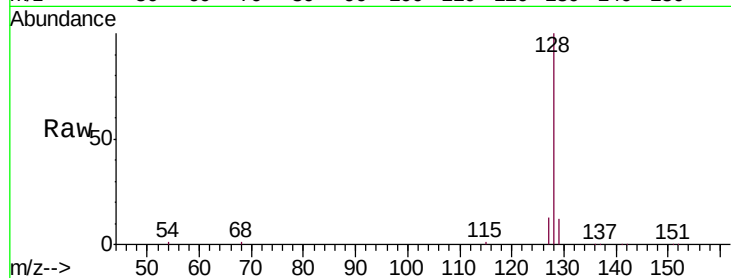

Abundance Ion 128.00 (127.70 to 128.70): E

Ion 129.00 (128.70 to 129.70): E

Ion 127.00 (126.70 to 127.70): E

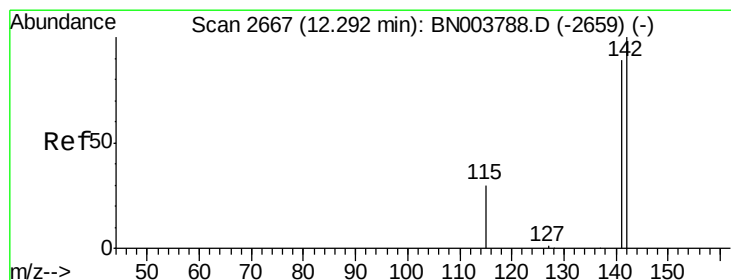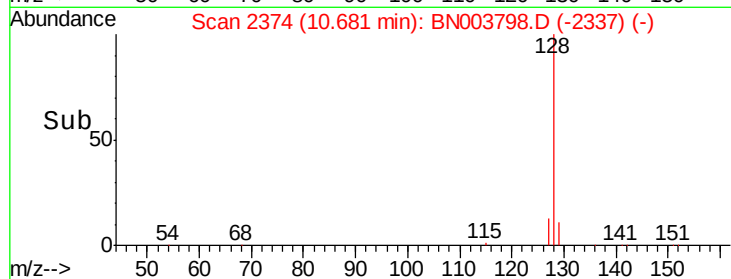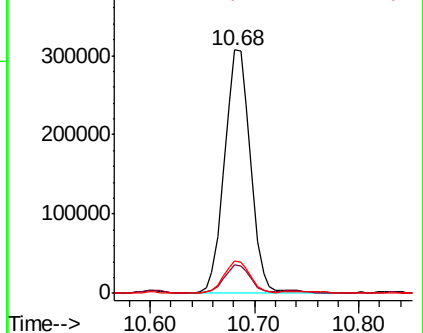

#5

2-Methylnaphthalene

Concen: 2.811 ng/ul

RT: 12.30 min Scan# 2668

Delta R.T. 0.01 min

Lab File: BN003798.D


Acq: 11 Dec 2018 03:04

Tgt Ion:142 Resp: 124794

Ion Ratio Lower Upper



142 100


141 89.2 71.5 107.3

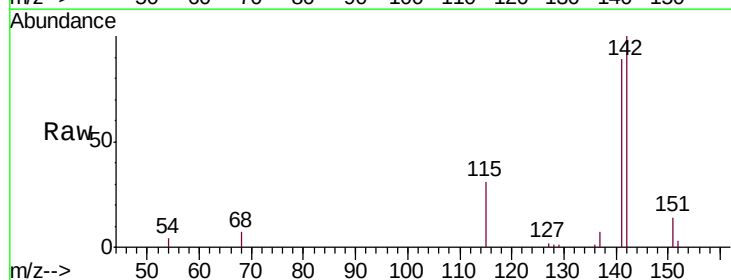

Abundance Ion 142.00 (141.70 to 142.70): E

Ion 141.00 (140.70 to 141.70): E

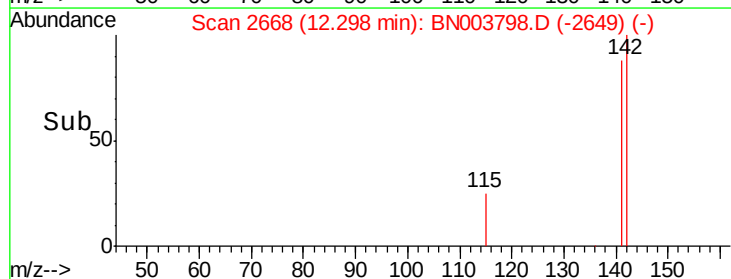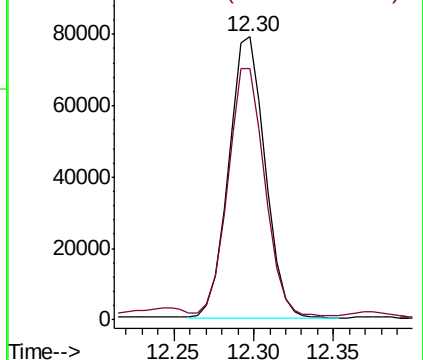

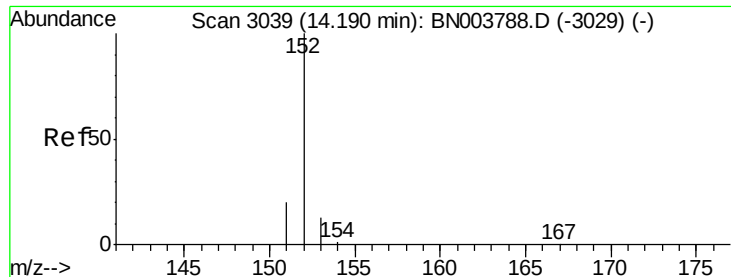

#7

Acenaphthylene

Concen: 0.188 ng/ul

RT: 14.20 min Scan# 3040

Delta R.T. 0.00 min

Lab File: BN003798.D

Acq: 11 Dec 2018 03:04

Instrument :

BNA_N

ClientSampleId :

F9Y32DL





Tgt Ion:152 Resp: 13217

Ion Ratio Lower Upper

152 100

151 79.8 15.9 23.9#

153 75.8 10.7 16.1#

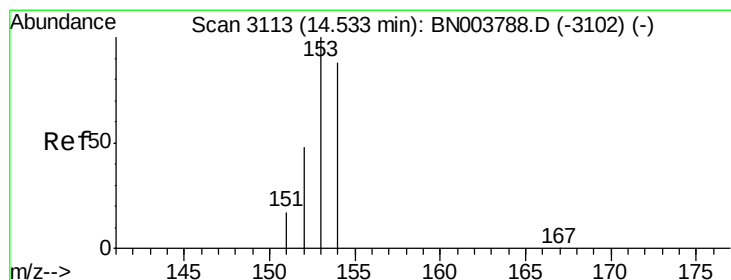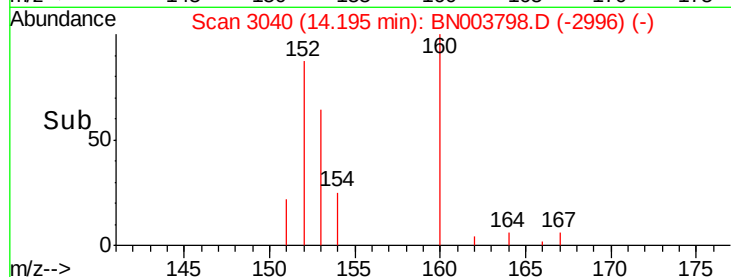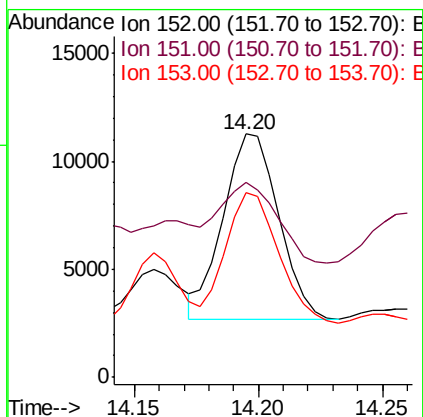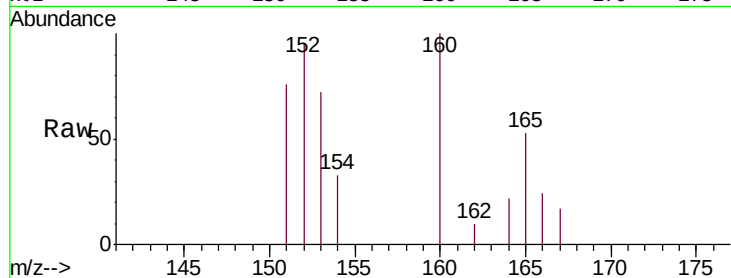

#8

Acenaphthene

Concen: 0.501 ng/ul

RT: 14.54 min Scan# 3115

Delta R.T. 0.01 min

Lab File: BN003798.D

Acq: 11 Dec 2018 03:04




Tgt Ion:153 Resp: 30924


Ion Ratio Lower Upper

153 100

152 60.6 39.3 58.9#

154 81.2 70.3 105.5


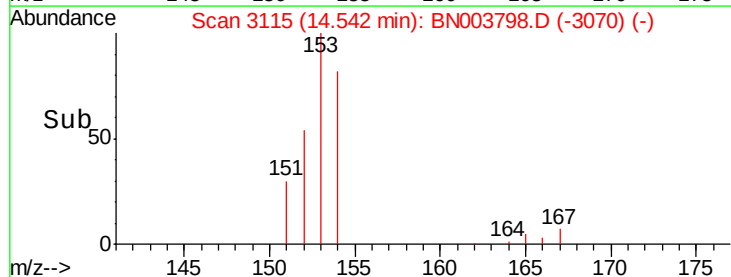
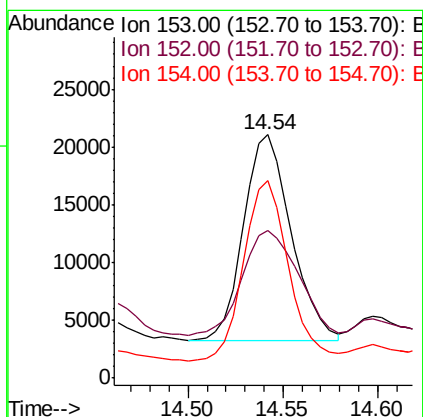
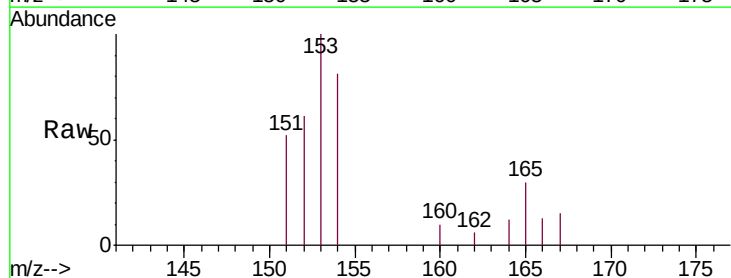


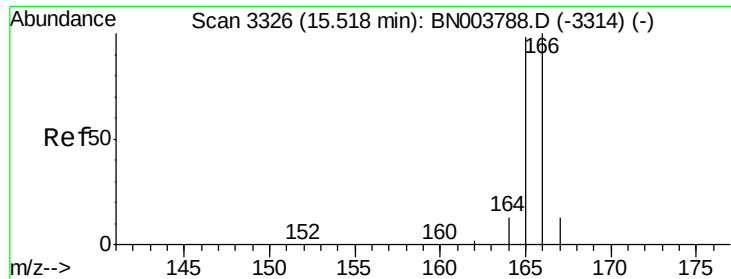

#9
Fluorene
 Concen: 0.478 ng/ul
 RT: 15.53 min Scan# 3328
 Delta R.T. 0.01 min
 Lab File: BN003798.D
 Acq: 11 Dec 2018 03:04




Instrument :
 BNA_N
 ClientSampleId :
 F9Y32DL


Tgt Ion:166 Resp: 34369
 Ion Ratio Lower Upper
 166 100
 165 116.9 78.3 117.5
 167 26.1 11.3 16.9#

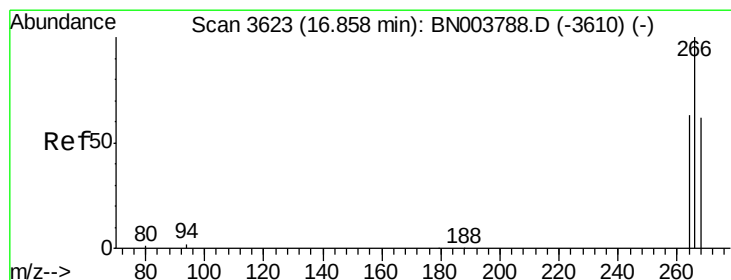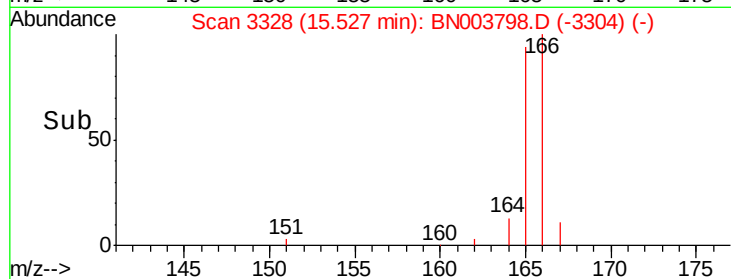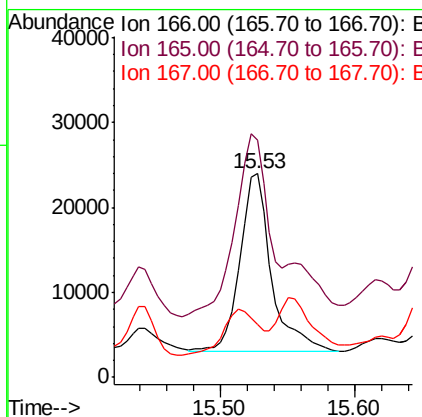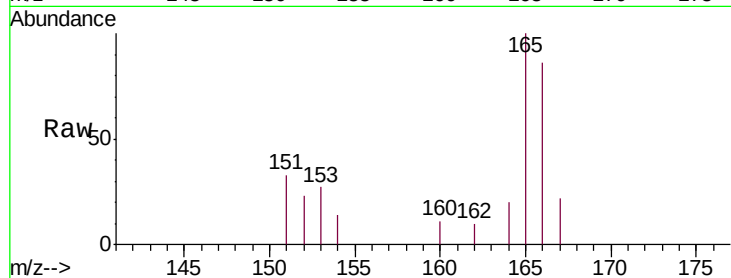

#11
Pentachlorophenol
 Concen: 0.157 ng/ul
 RT: 16.87 min Scan# 3625
 Delta R.T. 0.01 min
 Lab File: BN003798.D
 Acq: 11 Dec 2018 03:04

Tgt Ion:266 Resp: 578
 Ion Ratio Lower Upper
 266 100
 264 0.0 49.4 74.2#
 268 9.7 51.7 77.5#

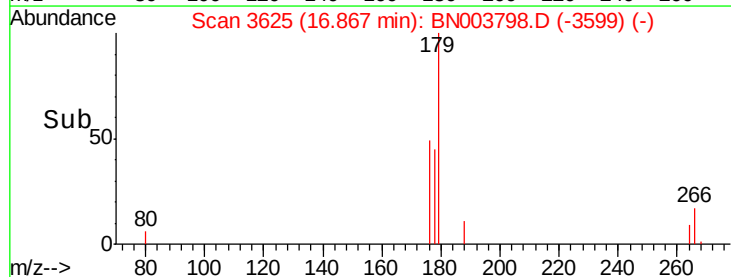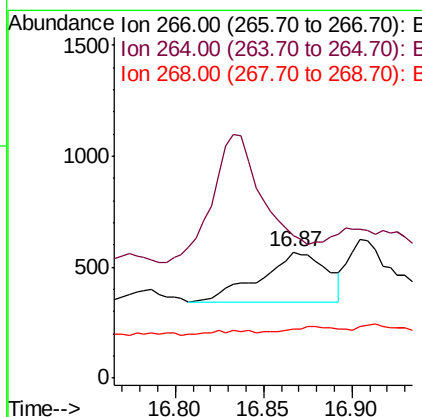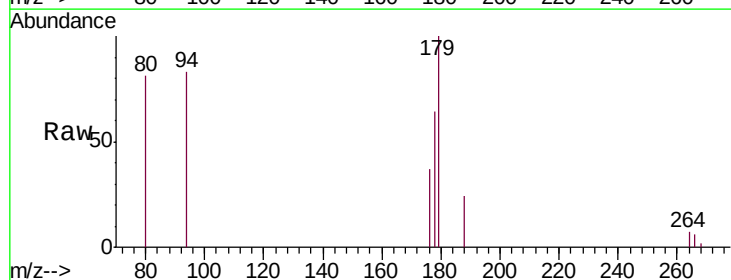

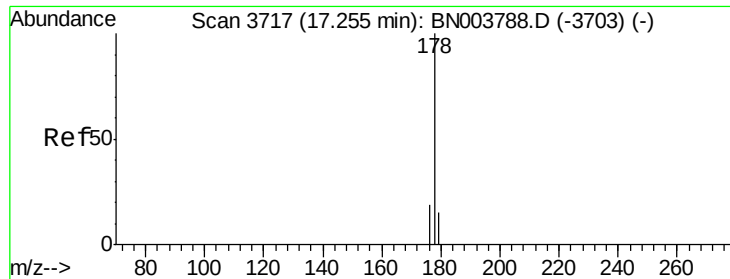

#12

Phenanthrene

Concen: 1.248 ng/ul

RT: 17.26 min Scan# 3719

Delta R.T. 0.01 min

Lab File: BN003798.D

Acq: 11 Dec 2018 03:04

Instrument :

BNA_N

ClientSampleId :

F9Y32DL





Tgt Ion:178 Resp: 83532

Ion Ratio Lower Upper

178 100

179 31.6 12.5 18.7#

176 21.8 15.0 22.4

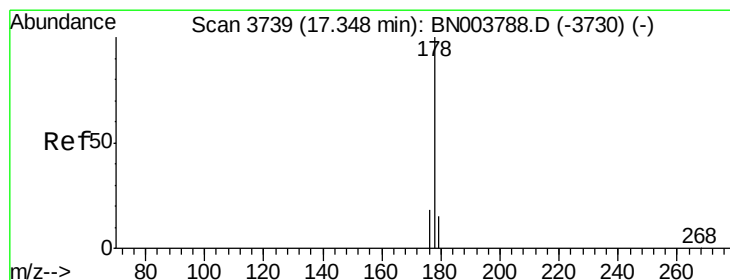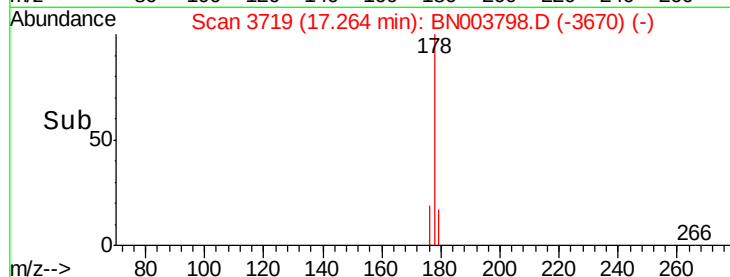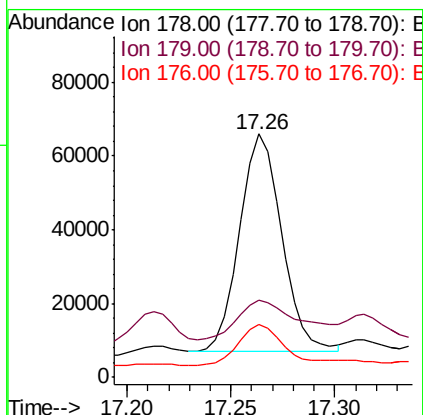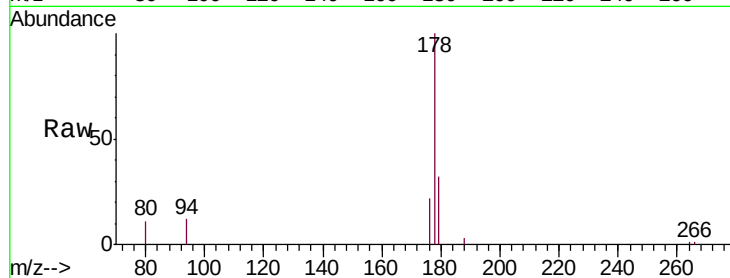

#13

Anthracene

Concen: 0.254 ng/ul

RT: 17.36 min Scan# 3741

Delta R.T. 0.01 min

Lab File: BN003798.D

Acq: 11 Dec 2018 03:04




Tgt Ion:178 Resp: 13968


Ion Ratio Lower Upper

178 100

179 58.2 12.3 18.5#

176 31.3 14.8 22.2#

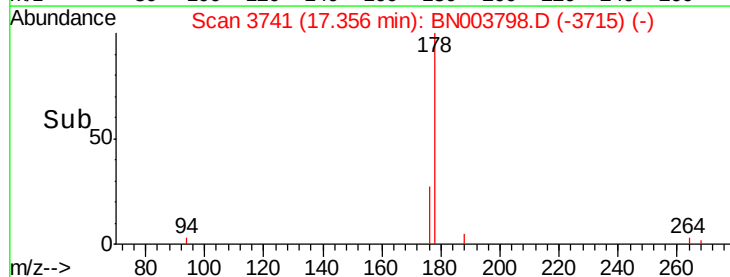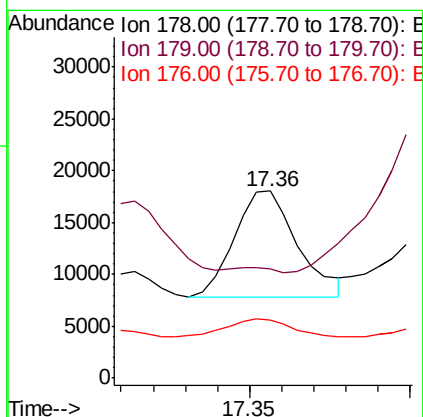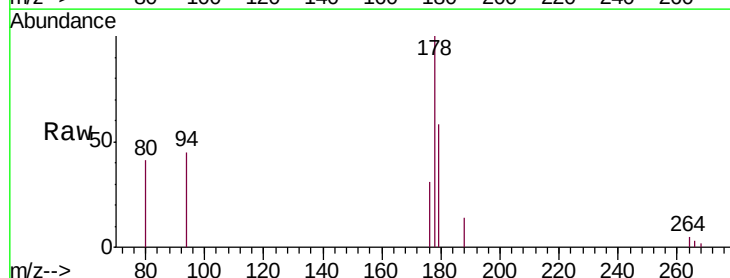


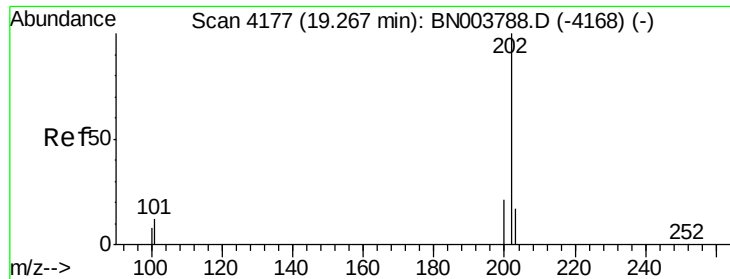




#15
Fluoranthene
 Concen: 0.418 ng/ul
 RT: 19.28 min Scan# 4179
 Delta R.T. 0.01 min
 Lab File: BN003798.D
 Acq: 11 Dec 2018 03:04

Instrument :
 BNA_N
 ClientSampleId :
 F9Y32DL

Tgt Ion	Ratio	Lower	Upper
202	100		
101	18.9	0.0	30.7
100	12.3	0.0	28.1

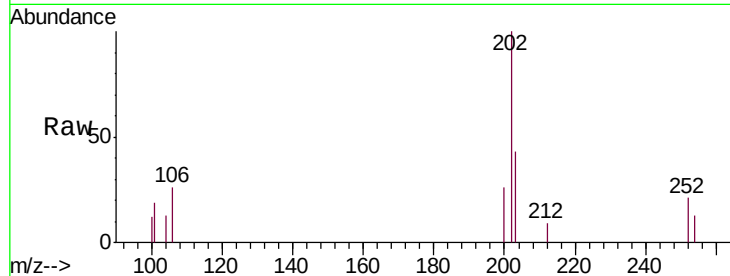


Abundance Ion 202.00 (201.70 to 202.70): E
 Ion 101.00 (100.70 to 101.70): E
 Ion 100.00 (99.70 to 100.70): B

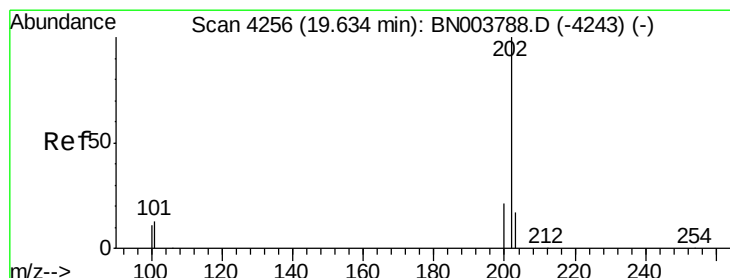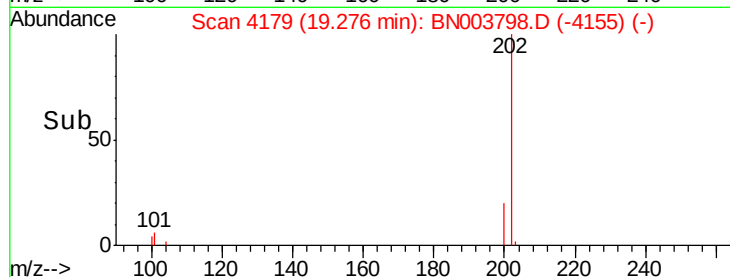
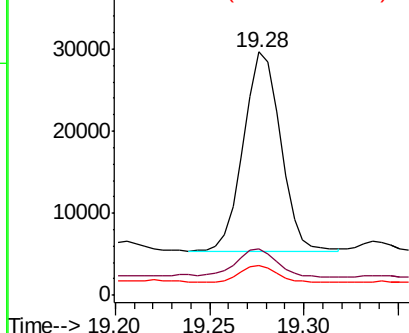



#17
Pyrene
 Concen: 1.234 ng/ul
 RT: 19.64 min Scan# 4258
 Delta R.T. 0.01 min
 Lab File: BN003798.D
 Acq: 11 Dec 2018 03:04

Tgt Ion	Ratio	Lower	Upper
202	100		
101	18.6	10.3	15.5#
100	12.6	8.5	12.7

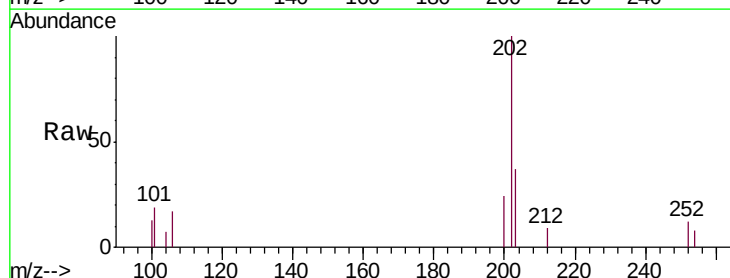

Abundance Ion 202.00 (201.70 to 202.70): E
 Ion 101.00 (100.70 to 101.70): E
 Ion 100.00 (99.70 to 100.70): B

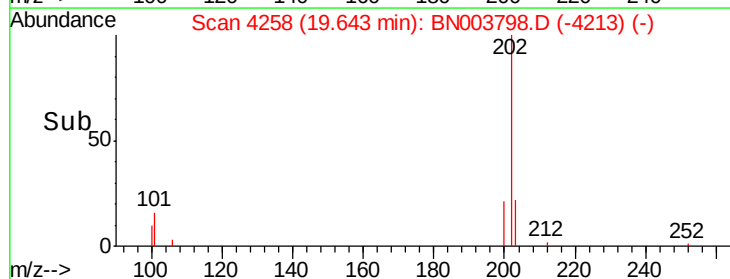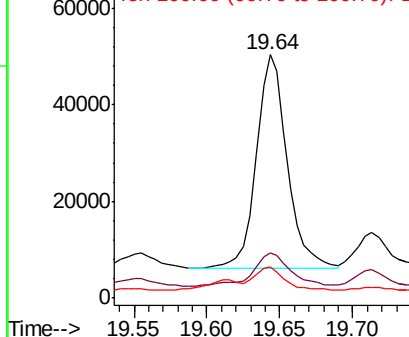

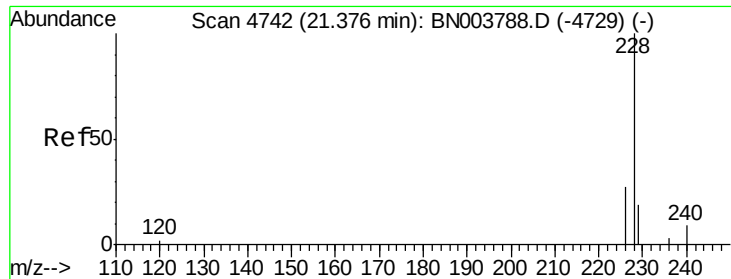

#18

Benzo(a)anthracene

Concen: 0.126 ng/ul

RT: 21.39 min Scan# 4746

Delta R.T. 0.01 min

Lab File: BN003798.D

Acq: 11 Dec 2018 03:04

Instrument :

BNA_N

ClientSampleId :

F9Y32DL


Tgt Ion:228 Resp: 5876

Ion Ratio Lower Upper




228 100

229 132.3 15.6 23.4#

226 71.7 21.1 31.7#

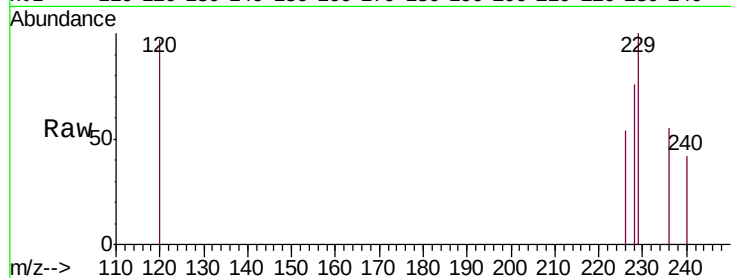

Abundance Ion 228.00 (227.70 to 228.70): E
Ion 229.00 (228.70 to 229.70): E
Ion 226.00 (225.70 to 226.70): E

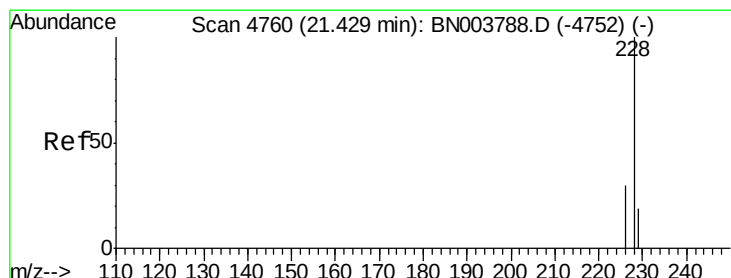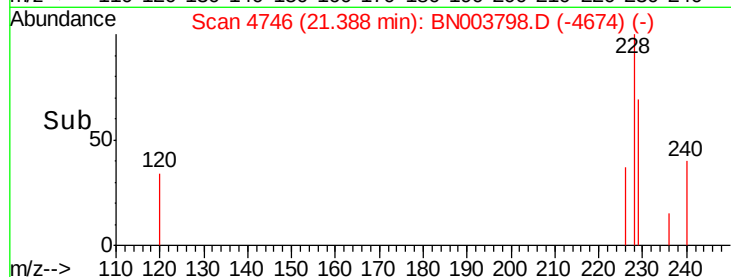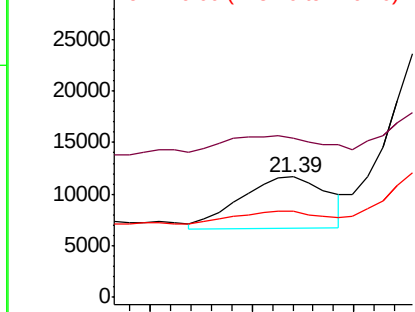

#19

Chrysene

Concen: 0.802 ng/ul

RT: 21.42 min Scan# 4756

Delta R.T. -0.01 min

Lab File: BN003798.D

Acq: 11 Dec 2018 03:04


Tgt Ion:228 Resp: 42765

Ion Ratio Lower Upper



228 100


226 46.3 24.0 36.0#

229 64.0 15.7 23.5#

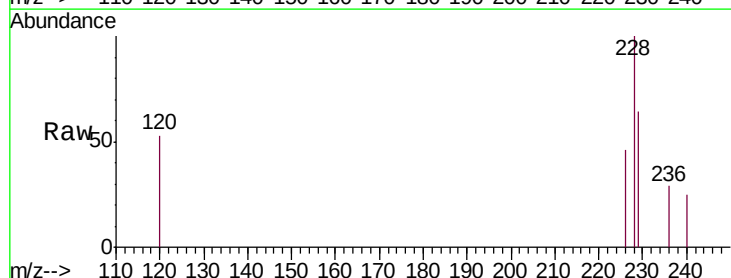

Abundance Ion 228.00 (227.70 to 228.70): E
Ion 226.00 (225.70 to 226.70): E
Ion 229.00 (228.70 to 229.70): E

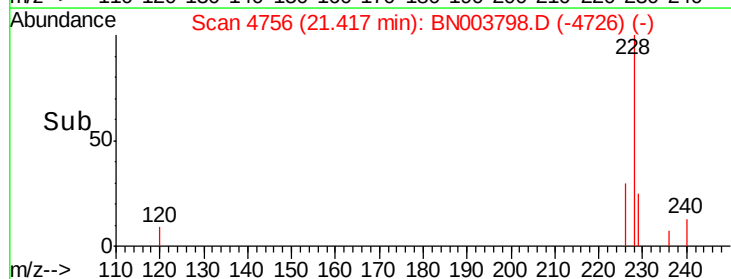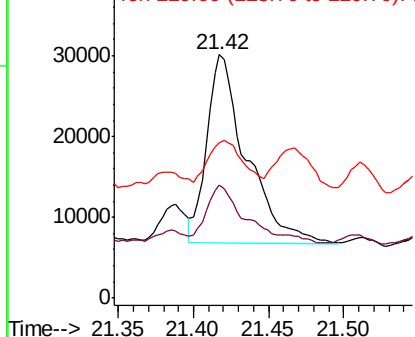

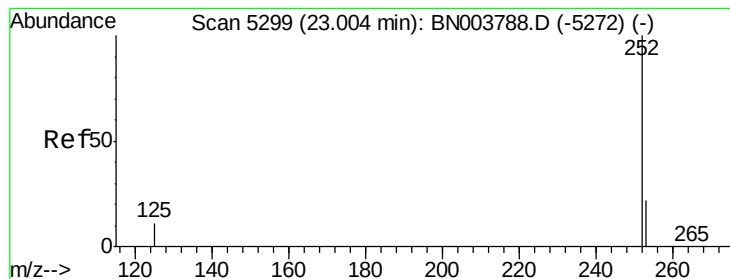

#21

Benzo(b)fluoranthene

Concen: 0.147 ng/ul

RT: 23.02 min Scan# 5304

Delta R.T. 0.01 min

Lab File: BN003798.D

Acq: 11 Dec 2018 03:04

Instrument :

BNA_N

ClientSampleId :

F9Y32DL


Tgt Ion:252 Resp: 10130

Ion Ratio Lower Upper

252 100

253 116.4 0.0 46.0#




125 584.1 0.0 22.4#

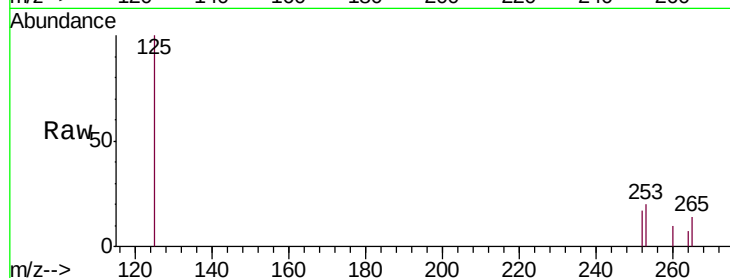

Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

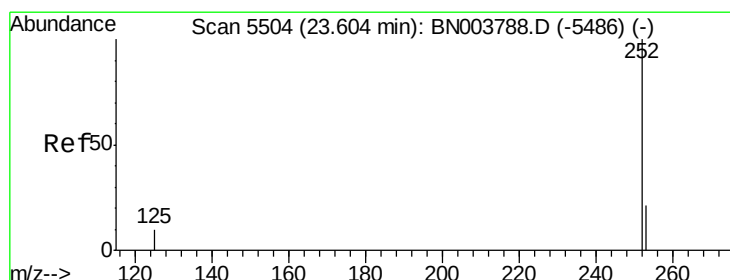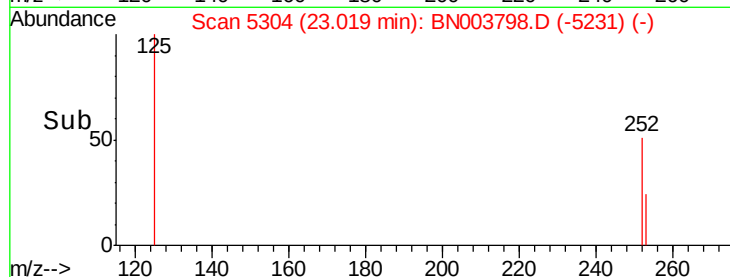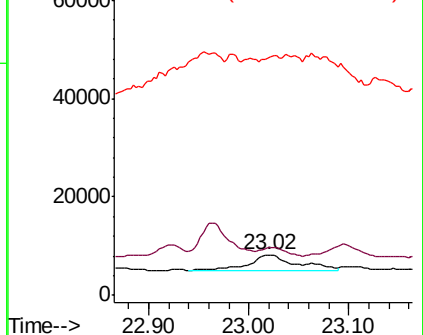

#23

Benzo(a)pyrene

Concen: 0.073 ng/ul

RT: 23.62 min Scan# 5510

Delta R.T. 0.02 min

Lab File: BN003798.D

Acq: 11 Dec 2018 03:04


Tgt Ion:252 Resp: 4357

Ion Ratio Lower Upper

252 100

253 108.3 19.0 28.4#



125 530.7 10.2 15.4#

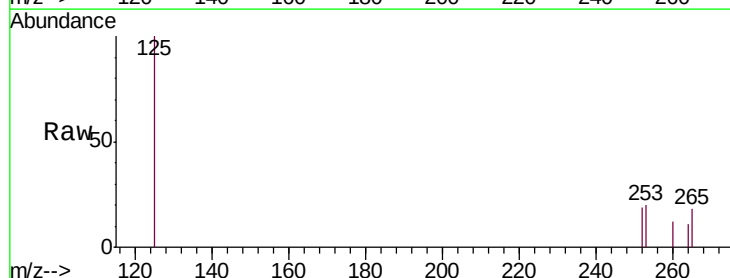


Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

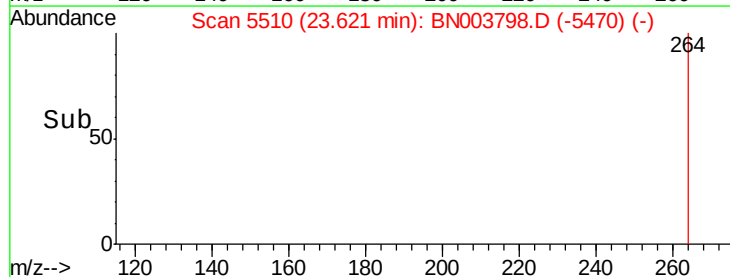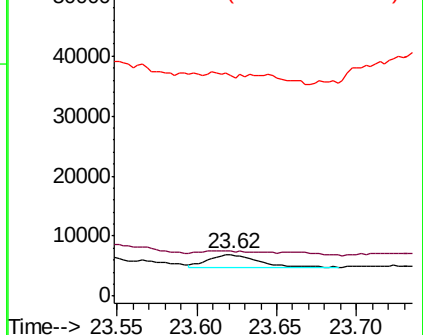

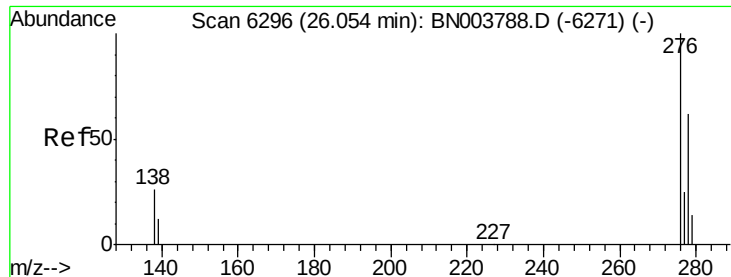

#24

Indeno(1,2,3-cd)pyrene

Concen: 0.036 ng/ul

RT: 26.08 min Scan# 6304

Delta R.T. 0.03 min

Lab File: BN003798.D

Acq: 11 Dec 2018 03:04

Instrument :

BNA_N

ClientSampleId :

F9Y32DL


Tgt Ion:276 Resp: 2469

Ion Ratio Lower Upper

276 100

138 0.0 20.3 30.5#

227 4.9 0.2 0.2#



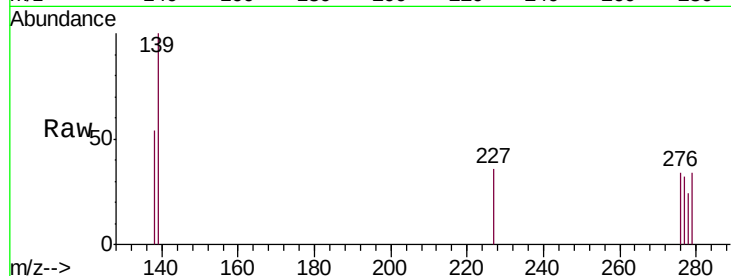


Abundance

Ion 276.00 (275.70 to 276.70): E

Ion 138.00 (137.70 to 138.70): E

Ion 227.00 (226.70 to 227.70): E

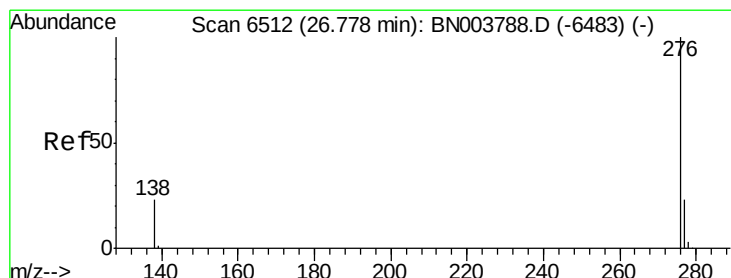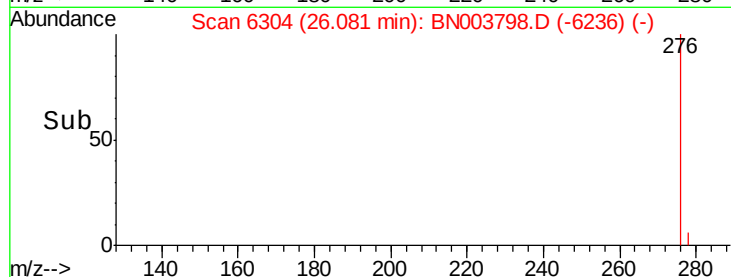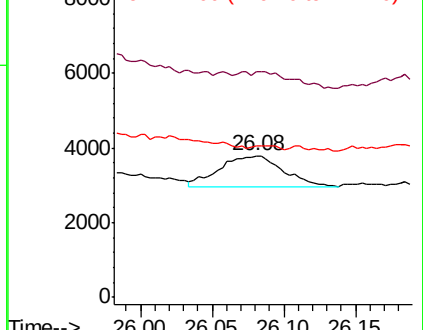

#26

Benzo(g,h,i)perylene

Concen: 0.123 ng/ul

RT: 26.81 min Scan# 6521

Delta R.T. 0.03 min

Lab File: BN003798.D

Acq: 11 Dec 2018 03:04


Tgt Ion:276 Resp: 7299

Ion Ratio Lower Upper

276 100

138 120.9 17.7 26.5#

277 79.5 19.3 28.9#

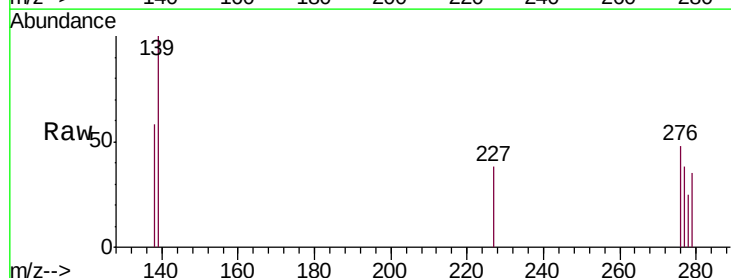

Abundance

Ion 276.00 (275.70 to 276.70): E

Ion 138.00 (137.70 to 138.70): E

Ion 277.00 (276.70 to 277.70): E

