

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN121018\
 Data File : BN003781.D
 Acq On : 10 Dec 2018 16:32
 Operator : JU/SJ
 Sample : J6155-14
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 A4118

Manual Integrations
 APPROVED

Sohil
 12/11/2018 6:12:14 PM

Quant Time: Dec 11 04:09:12 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN111918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Dec 11 03:42:06 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.84	152	4979	0.40	ng/ul	0.00
2) Naphthalene-d8	10.63	136	20676	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.47	164	11649	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.21	188	23923m	0.40	ng/ul	0.00
16) Chrysene-d12	21.40	240	18473m	0.40	ng/ul	0.00
20) Perylene-d12	23.72	264	14225m	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.22	152	10527	0.33	ng/ul	0.00
14) Fluoranthene-d10	19.24	212	22283m	0.32	ng/ul	0.00
Target Compounds						
8) Acenaphthene	14.54	153	4566	0.099	ng/ul#	Ovalue 24

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN121018\
Data File : BN003781.D
Acq On : 10 Dec 2018 16:32
Operator : JU/SJ
Sample : J6155-14
Misc :
ALS Vial : 8 Sample Multiplier: 1




Instrument :
BNA_N
ClientSampleId :
A4118

Manual Integrations
APPROVED

Sohil
12/11/2018 6:12:14 PM

Quant Time: Dec 11 04:09:12 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 11 03:42:06 2018
Response via : Initial Calibration

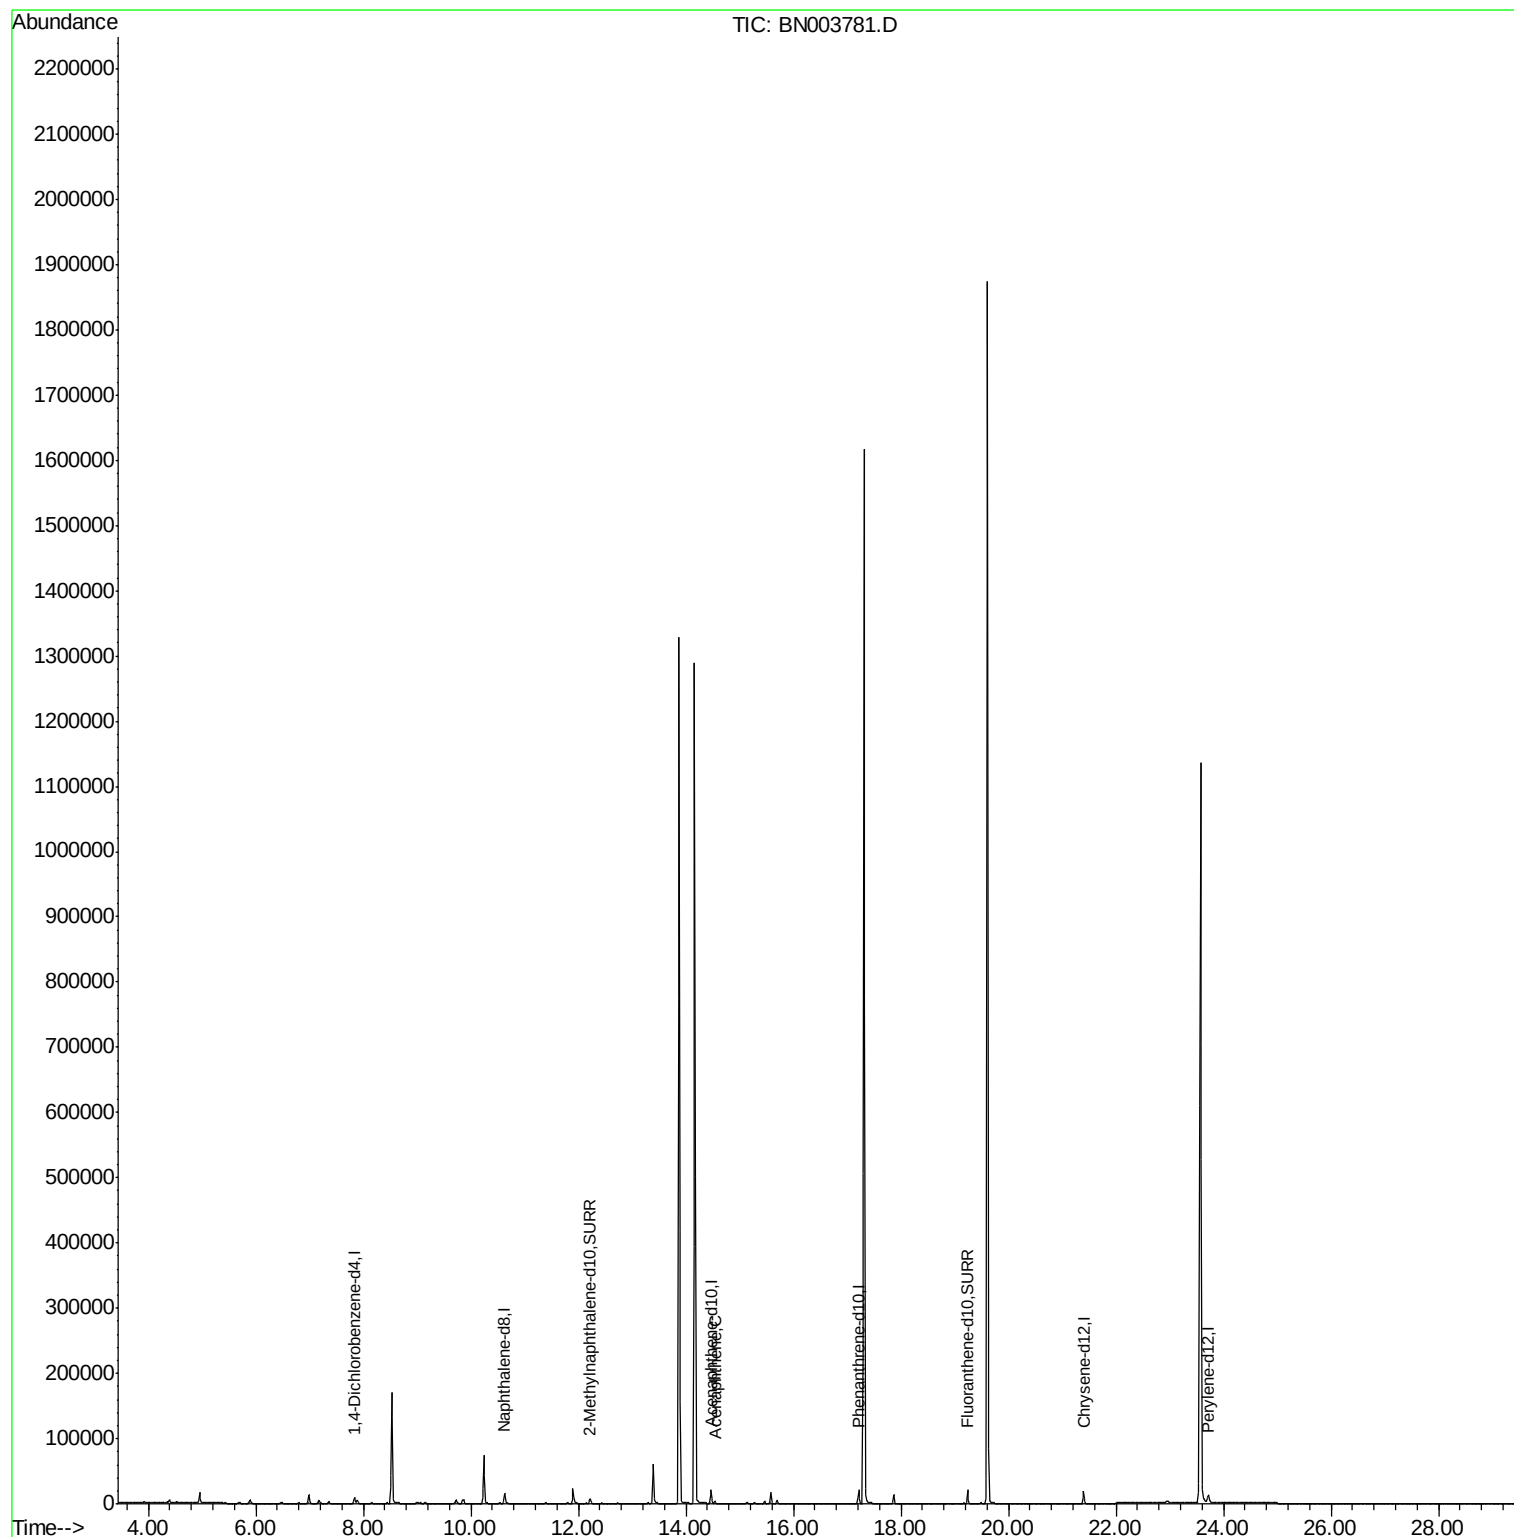

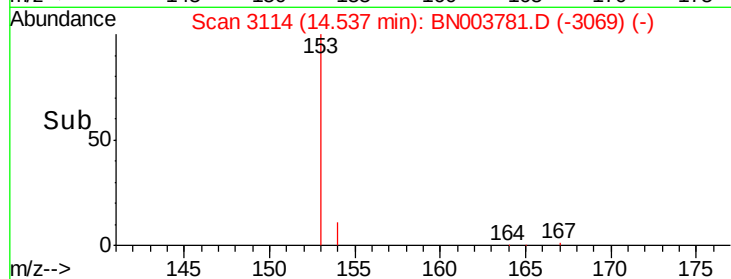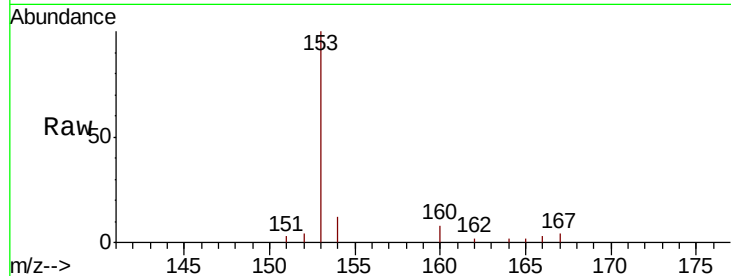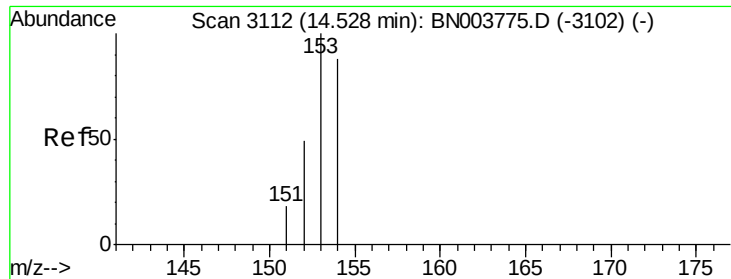

#8

Acenaphthene

Concen: 0.099 ng/ul

RT: 14.54 min Scan# 3114

Delta R.T. 0.01 min

Lab File: BN003781.D

Acq: 10 Dec 2018 16:32

Instrument :

BNA_N

ClientSampleId :

A4118

Tot Ion:153 Resp: 4566

Ion Ratio Lower Upper

153 100

152 3.7 39.3 58.9#

154 12.1 70.3 105.5#

Manual Integrations

APPROVED

Sohil

12/11/2018 6:12:14 PM

