

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN121018\
 Data File : BN003785.D
 Acq On : 10 Dec 2018 18:53
 Operator : JU/SJ
 Sample : J6155-19
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 A4168

Manual Integrations
 APPROVED

Sohil
 12/11/2018 6:12:16 PM

Quant Time: Dec 11 04:18:52 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN111918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Dec 11 03:42:06 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.84	152	5250	0.40	ng/ul	0.00
2) Naphthalene-d8	10.63	136	21881	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.47	164	12237	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.21	188	25582m	0.40	ng/ul	0.00
16) Chrysene-d12	21.39	240	20992m	0.40	ng/ul	0.00
20) Perylene-d12	23.71	264	15802m	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.22	152	10349	0.31	ng/ul	0.00
14) Fluoranthene-d10	19.24	212	23315m	0.31	ng/ul	0.00
Target Compounds						
3) Naphthalene	10.68	128	1616	0.026	ng/ul#	Ovalue 87

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN121018\
Data File : BN003785.D
Acq On : 10 Dec 2018 18:53
Operator : JU/SJ
Sample : J6155-19
Misc :
ALS Vial : 12 Sample Multiplier: 1




Instrument :
BNA_N
ClientSampleId :
A4168

Quant Time: Dec 11 04:18:52 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 11 03:42:06 2018
Response via : Initial Calibration

Manual Integrations
APPROVED

Sohil
12/11/2018 6:12:16 PM

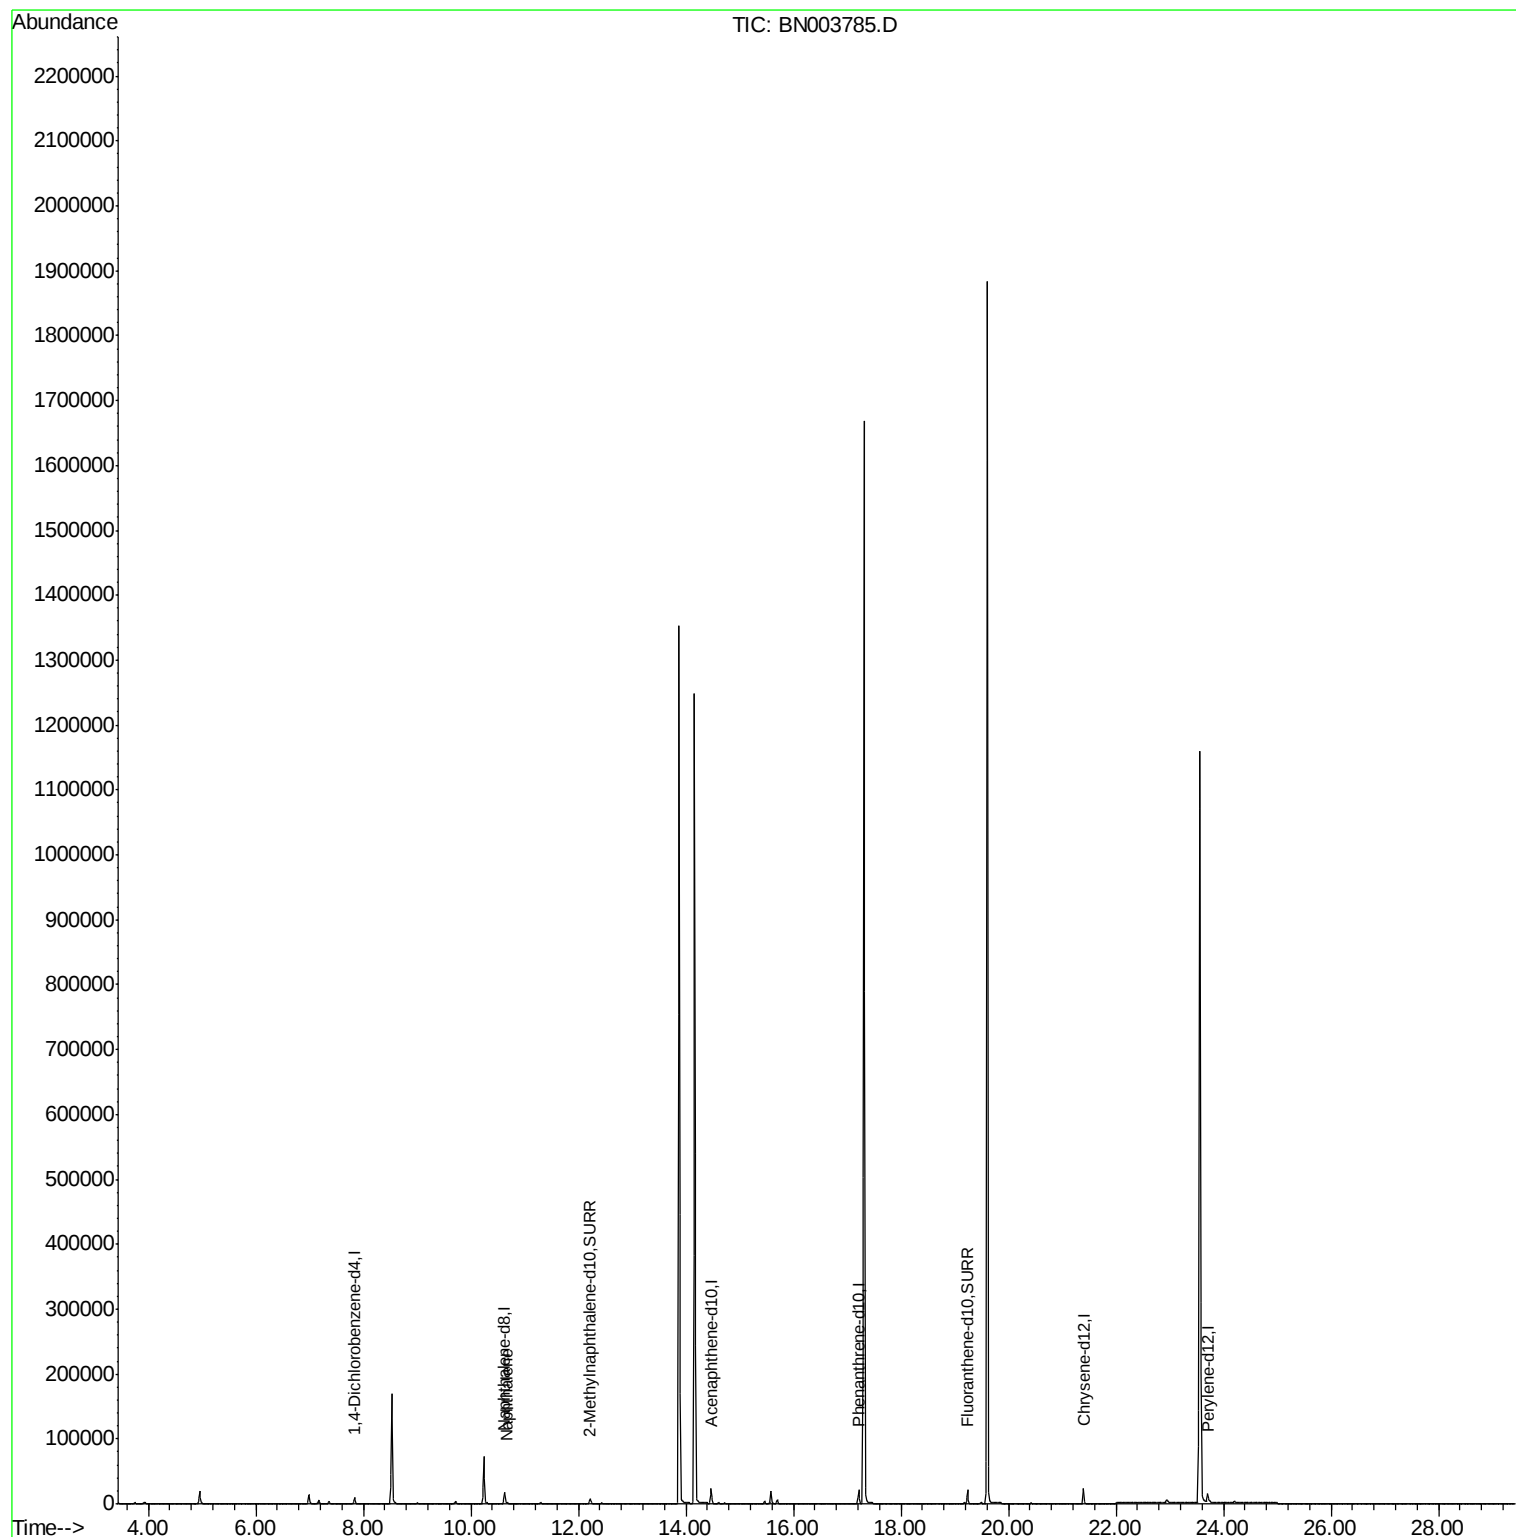

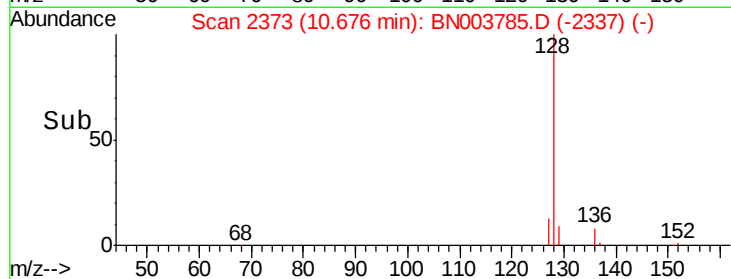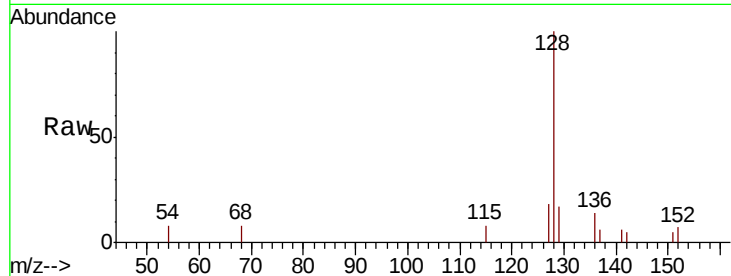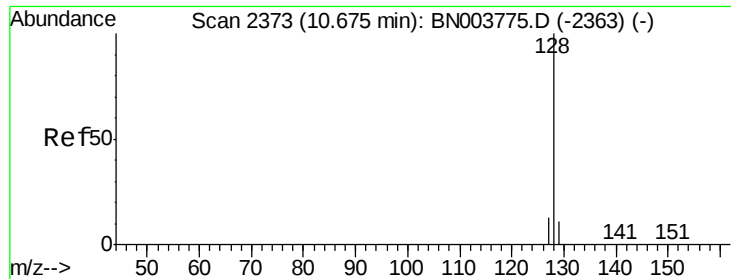

#3

Naphthalene

Concen: 0.026 ng/ul

RT: 10.68 min Scan# 2373

Delta R.T. 0.00 min

Lab File: BN003785.D

Acq: 10 Dec 2018 18:53

Instrument :

BNA_N

ClientSampleId :

A4168

Tot Ion:128 Resp: 1616

Ion Ratio Lower Upper

128 100

129 17.3 9.0 13.6#

127 17.6 10.5 15.7#

Manual Integrations

APPROVED

Sohil

12/11/2018 6:12:16 PM

