

Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN121018\
 Data File : BN003786.D
 Acq On : 10 Dec 2018 19:29
 Operator : JU/SJ
 Sample : J6155-20
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 A4170

Manual Integrations
 APPROVED

Sohil
 12/11/2018 6:12:17 PM

Quant Time: Dec 11 04:22:08 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN111918.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Dec 11 03:42:06 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.84	152	5203	0.40	ng/ul	0.00
2) Naphthalene-d8	10.63	136	21425	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.47	164	12133	0.40	ng/ul	0.00
10) Phenanthrene-d10	17.21	188	24856m	0.40	ng/ul	0.00
16) Chrysene-d12	21.39	240	20920m	0.40	ng/ul	0.00
20) Perylene-d12	23.71	264	16073m	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	12.22	152	9723	0.30	ng/ul	0.00
14) Fluoranthene-d10	19.24	212	21554m	0.30	ng/ul	0.00
Target Compounds						
12) Phenanthrene	17.25	178	2316	0.028	ng/ul	93

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\SVOASRV\HPCHEM1\BNA N\DATA\BN121018\
Data File : BN003786.D
Acq On : 10 Dec 2018 19:29
Operator : JU/SJ
Sample : J6155-20
Misc :
ALS Vial : 13 Sample Multiplier: 1




Instrument :
BNA_N
ClientSampleId :
A4170

Quant Time: Dec 11 04:22:08 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA N\METHODS\SOM-EPA-SIM-BN111918.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 11 03:42:06 2018
Response via : Initial Calibration

Manual Integrations
APPROVED

Sohil
12/11/2018 6:12:17 PM

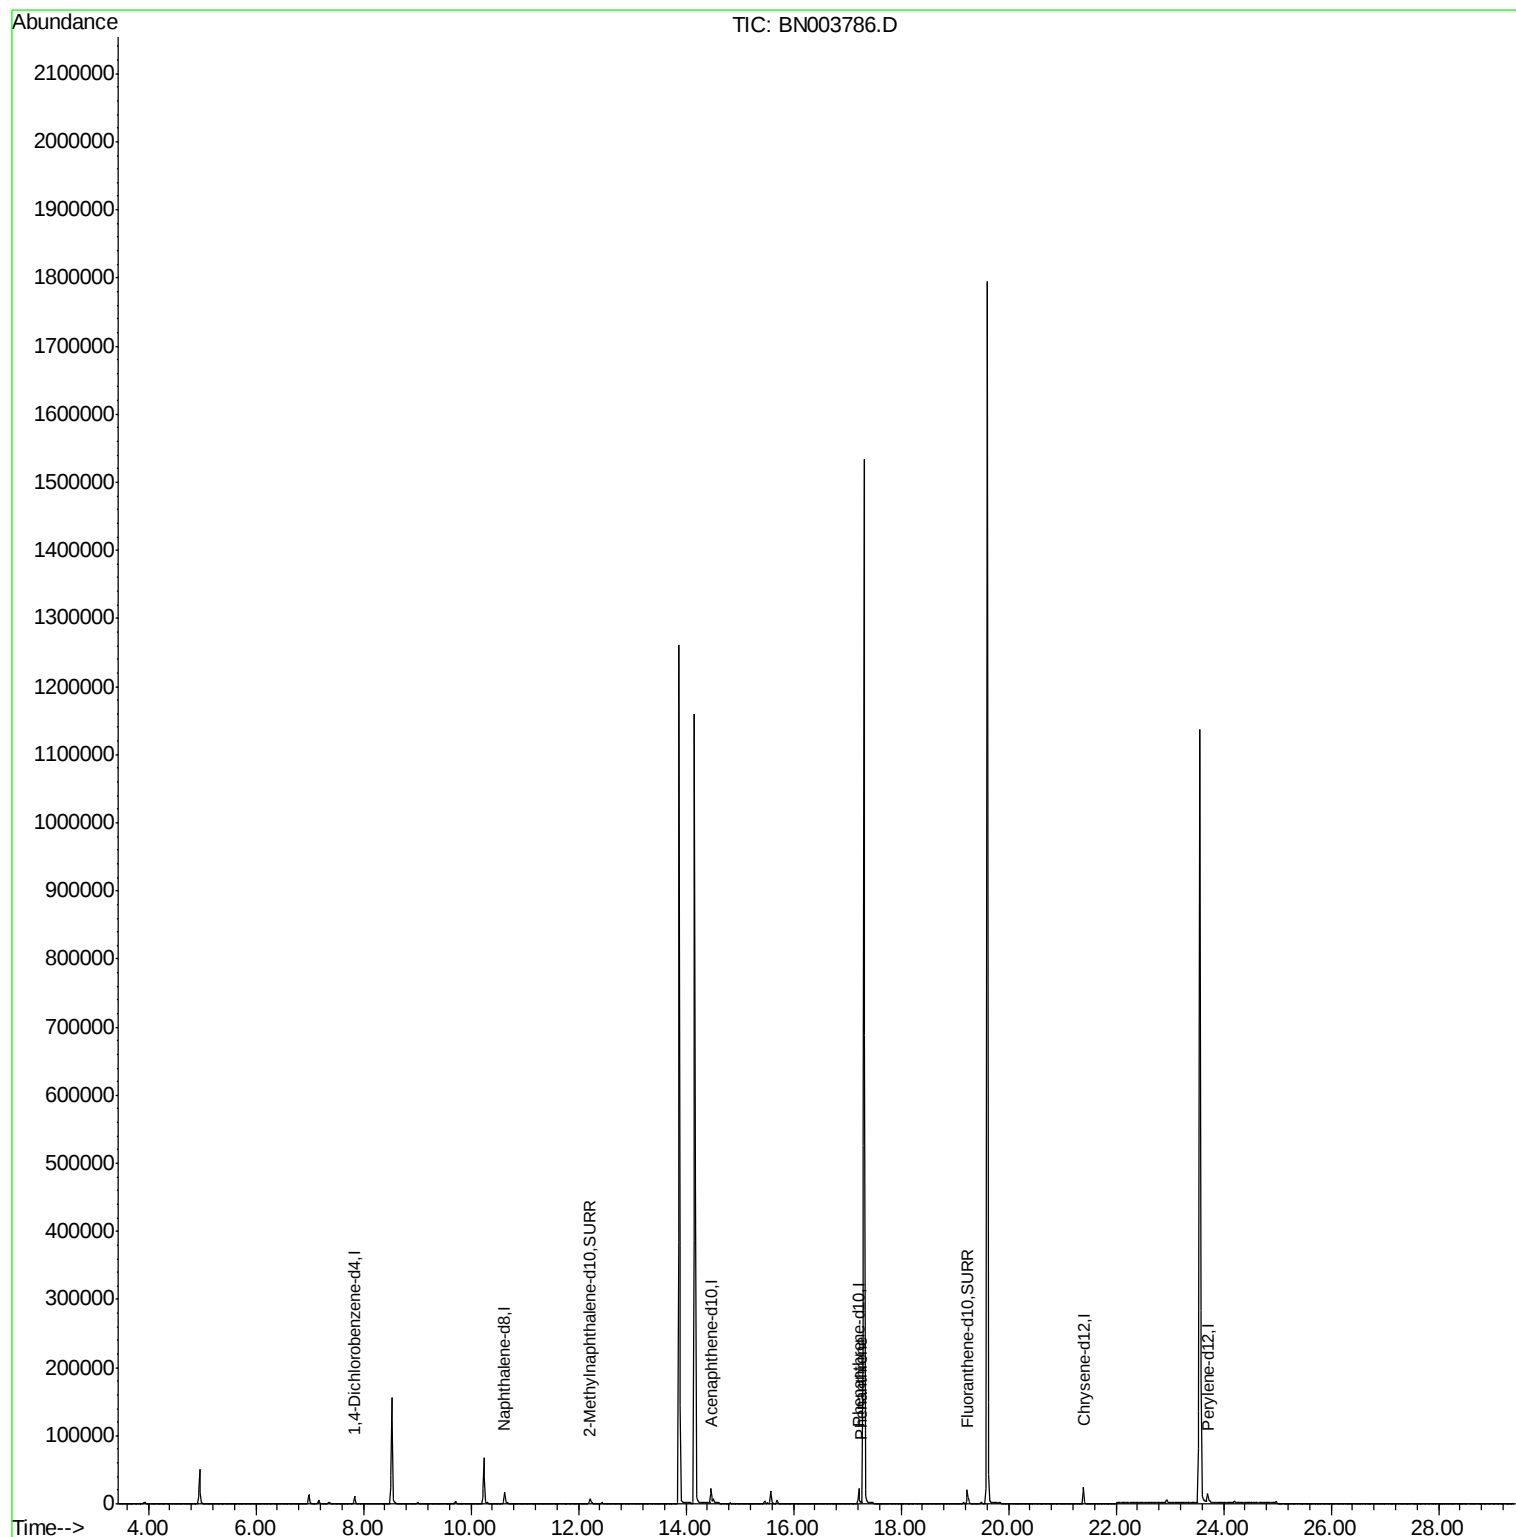

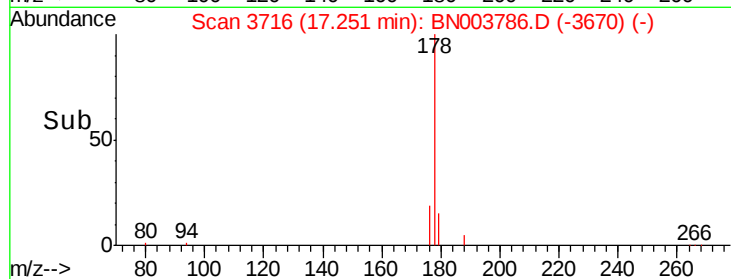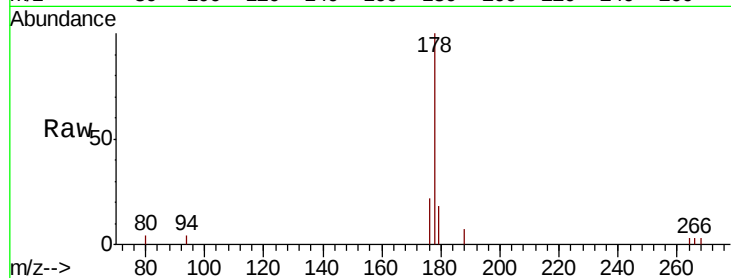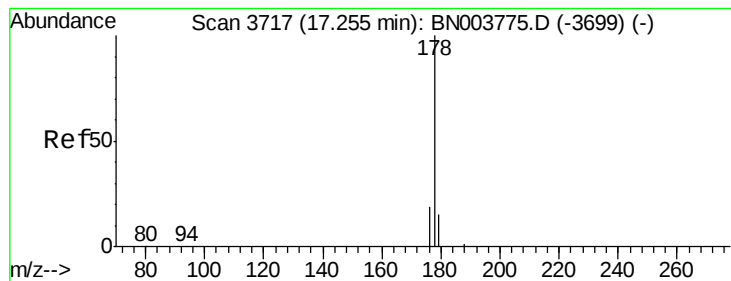

#12

Phenanthrene

Concen: 0.028 ng/ul

RT: 17.25 min Scan# 3716

Delta R.T. -0.00 min

Lab File: BN003786.D

Acq: 10 Dec 2018 19:29

Instrument :

BNA_N

ClientSampleId :

A4170

Tot Ion:	178	Resp:	2316
Ion Ratio	Lower	Upper	
178	100		
179	18.5	12.5	18.7
176	21.7	15.0	22.4

Manual Integrations
APPROVED

Sohil
12/11/2018 6:12:17 PM

