
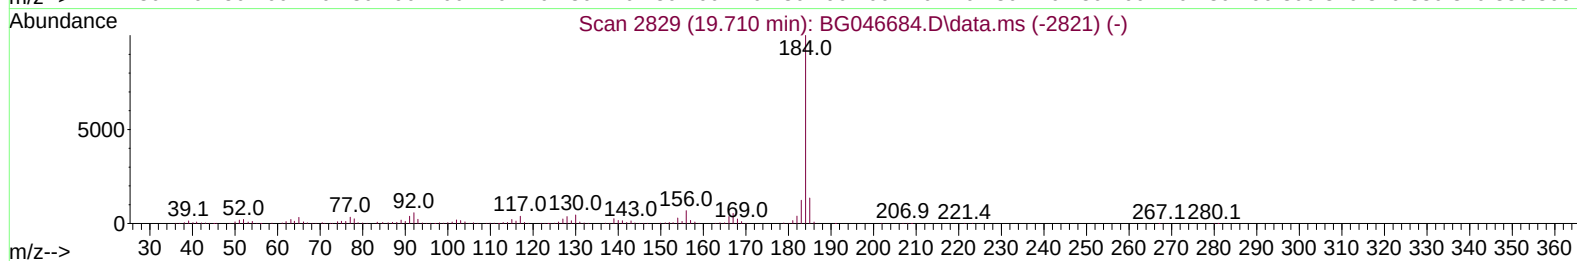
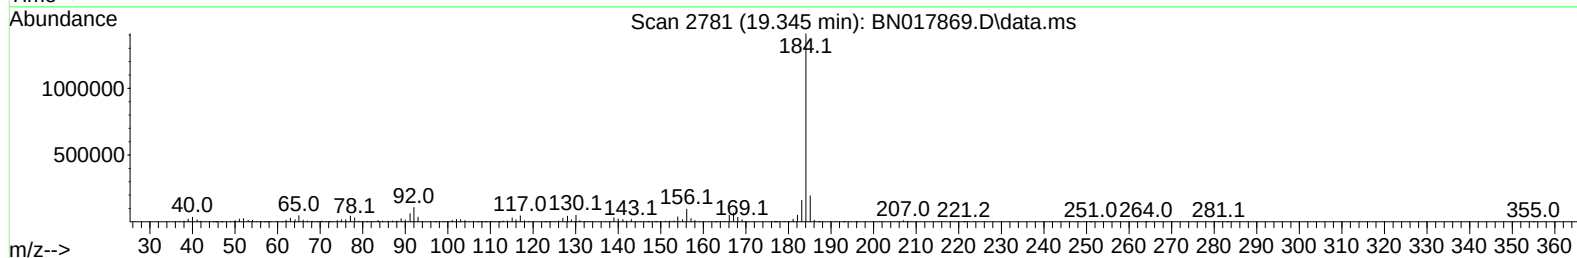


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121021\
Data File : BN017869.D
Acq On : 10 Dec 2021 13:59
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 11 07:40:04 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Dec 11 07:39:58 2021
Response via : Initial Calibration

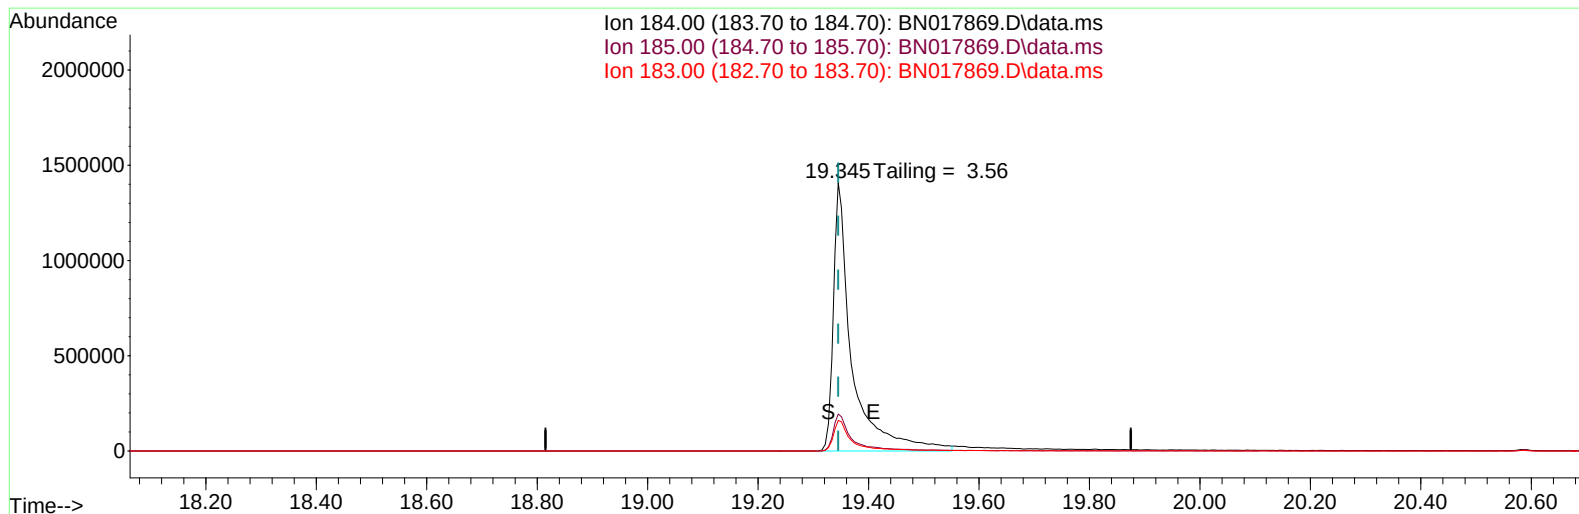

TIC: BN017869.D\data.ms

(77) Benzidine




19.345min (0.000) 0.00 ng

response 3439254

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.80
183.00	13.20	11.39
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121021\
Data File : BN017869.D
Acq On : 10 Dec 2021 13:59
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 11 07:40:04 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Dec 11 07:39:58 2021
Response via : Initial Calibration

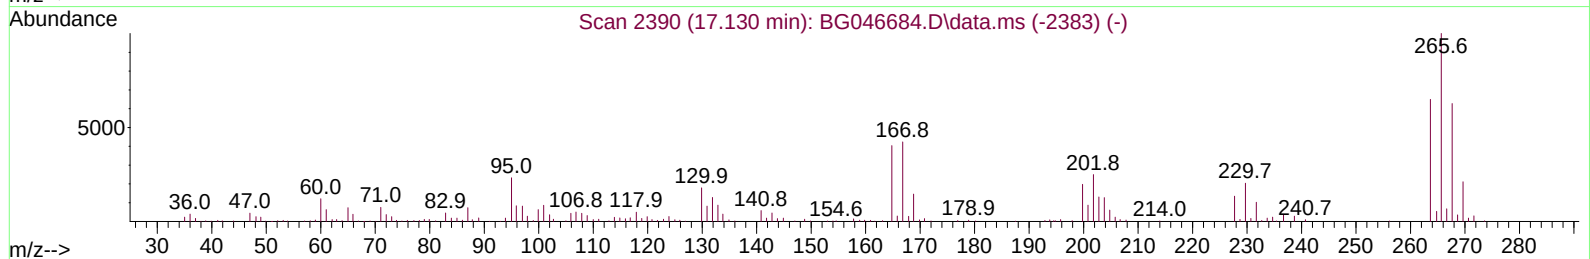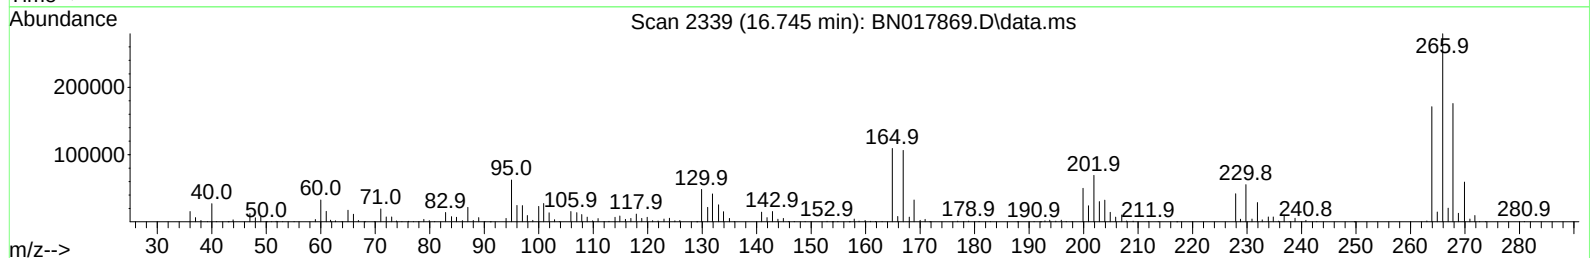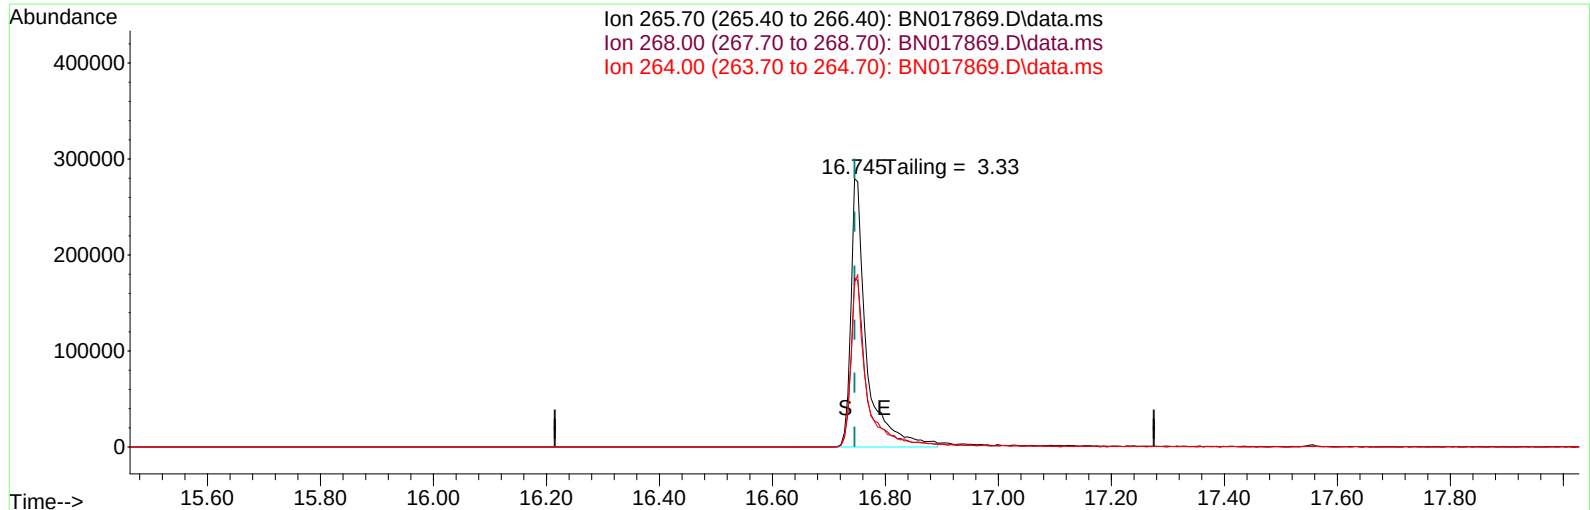

TIC: BN017869.D\data.ms

(70) Pentachlorophenol (C)

16.745min (0.000) 14903.35 ng

response 550988

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	62.93
264.00	61.60	61.24
0.00	0.00	0.00