
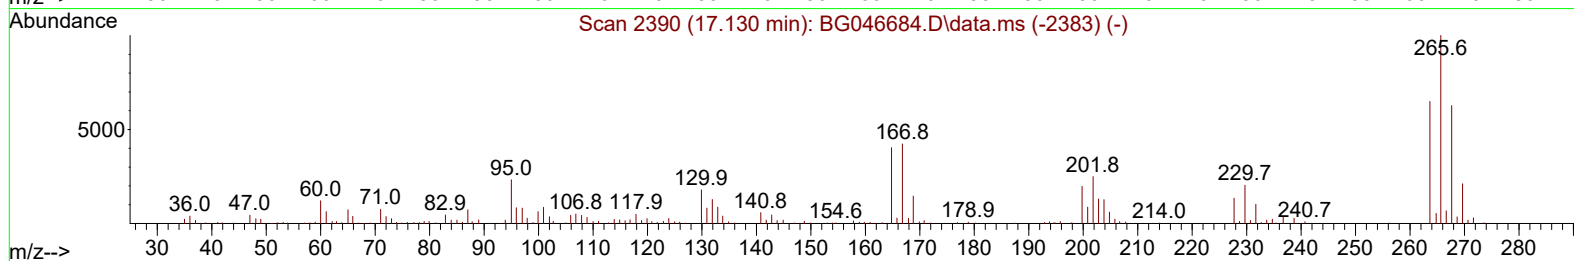
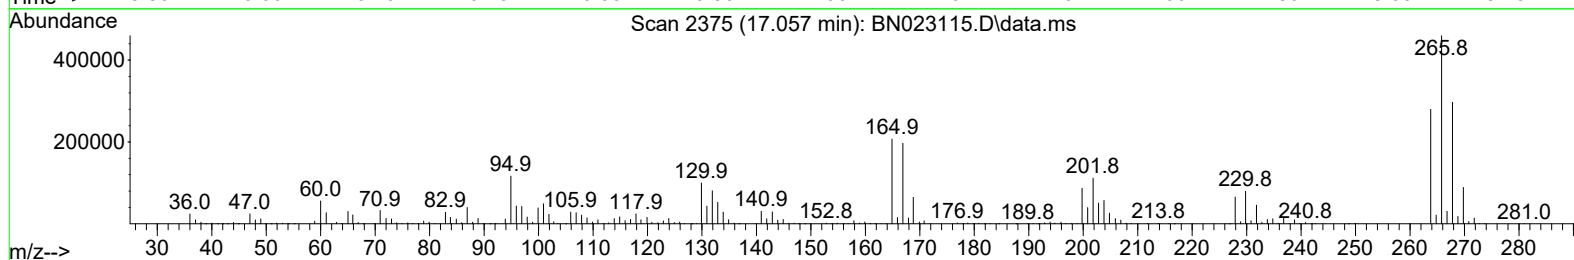


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121022\
Data File : BN023115.D
Acq On : 10 Dec 2022 09:44
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 12 07:11:29 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 12 07:11:25 2022
Response via : Initial Calibration

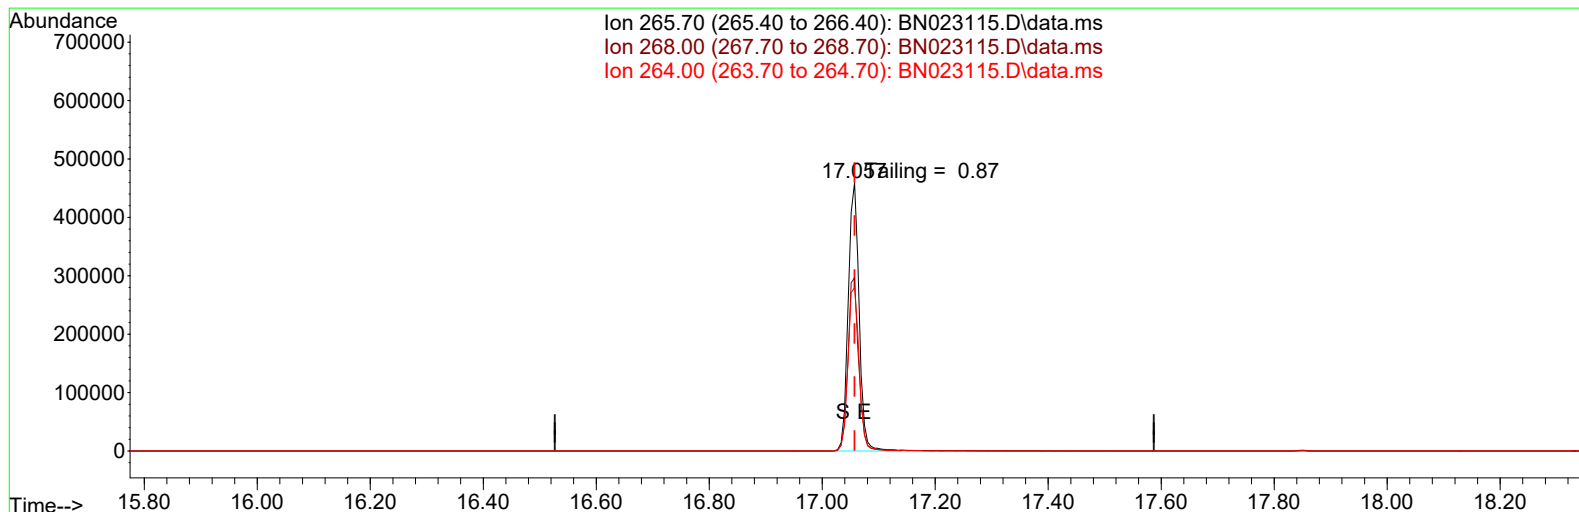

TIC: BN023115.D\data.ms

(70) Pentachlorophenol (C)




17.057min (0.000) 18995.35 ng

response 617302

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	64.57
264.00	61.60	60.89
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121022\
Data File : BN023115.D
Acq On : 10 Dec 2022 09:44
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 12 07:11:29 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 12 07:11:25 2022
Response via : Initial Calibration

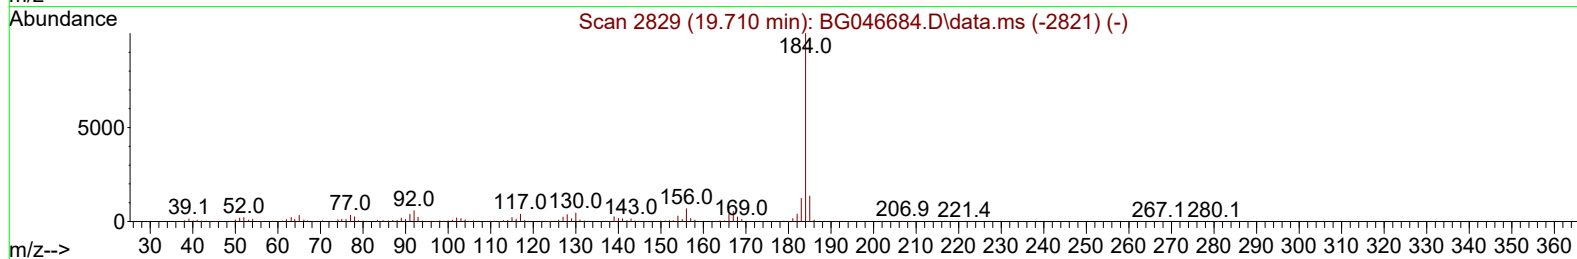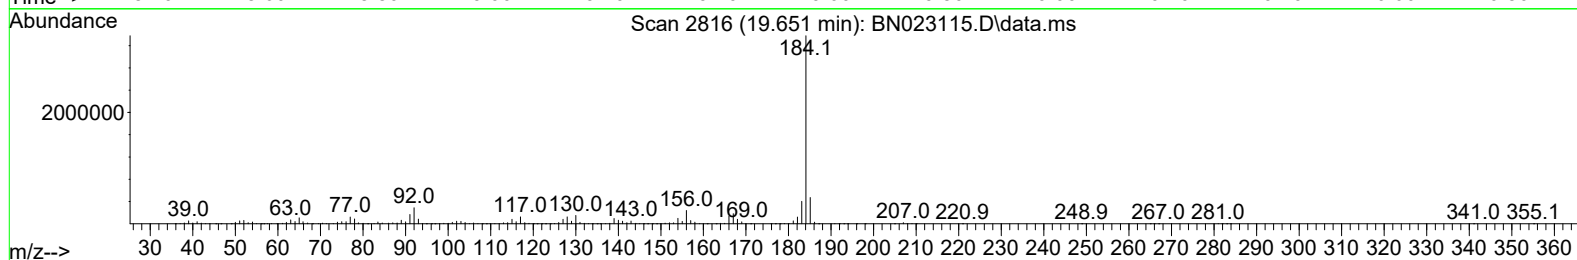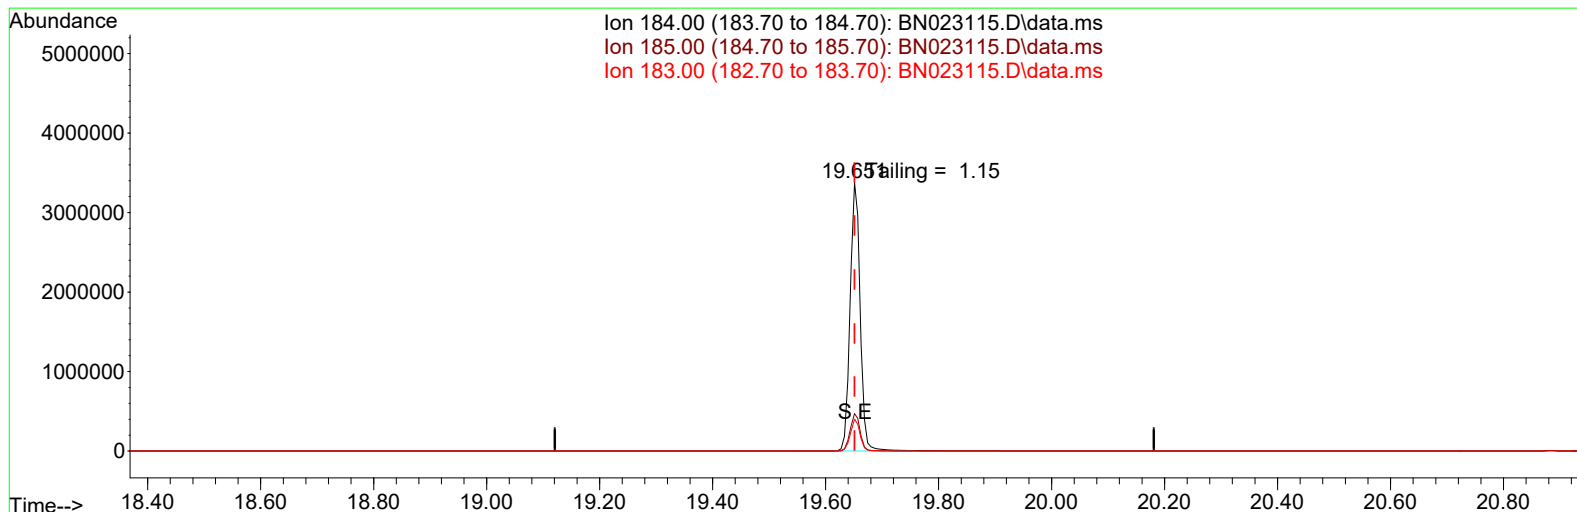

TIC: BN023115.D\data.ms

(77) Benzidine

19.651min (0.000) 0.00 ng

response 4209687

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.98
183.00	13.20	11.89
0.00	0.00	0.00