
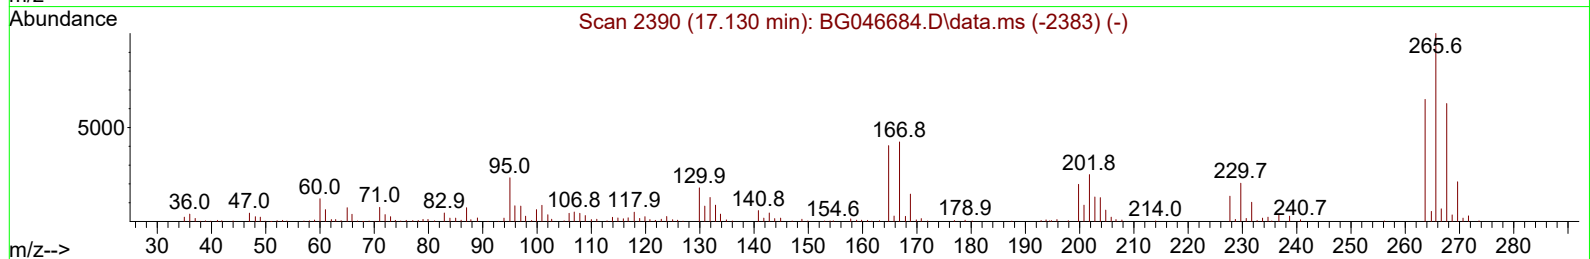
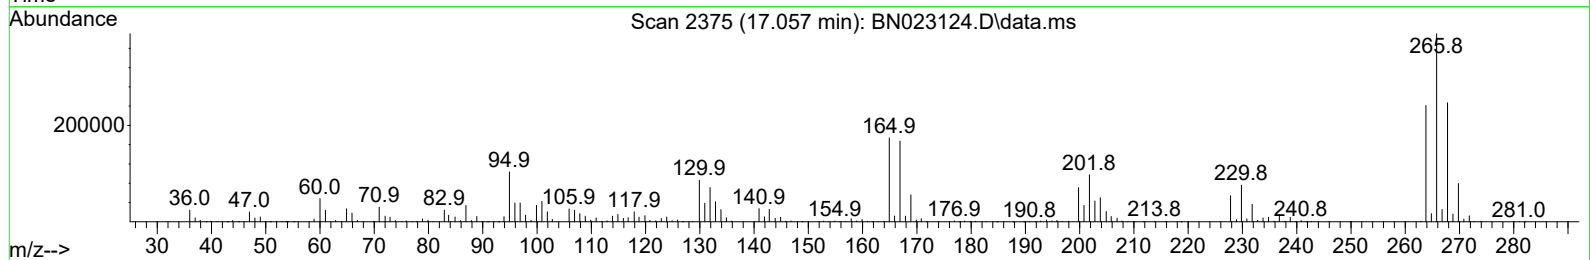


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121022\
Data File : BN023124.D
Acq On : 10 Dec 2022 16:34
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 12 07:12:41 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 12 07:11:25 2022
Response via : Initial Calibration

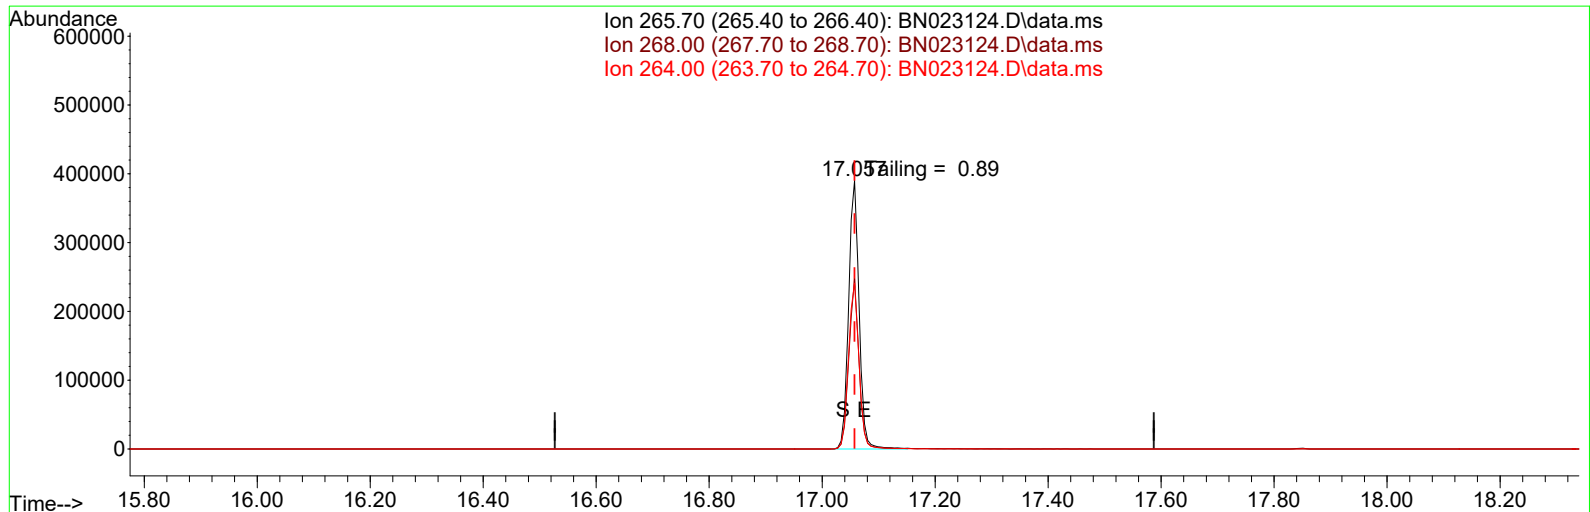

TIC: BN023124.D\data.ms

(70) Pentachlorophenol (C)




17.057min (+ 0.000) 19581.30 ng

response 505725

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	63.35
264.00	61.60	61.86
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121022\
Data File : BN023124.D
Acq On : 10 Dec 2022 16:34
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 12 07:12:41 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 12 07:11:25 2022
Response via : Initial Calibration

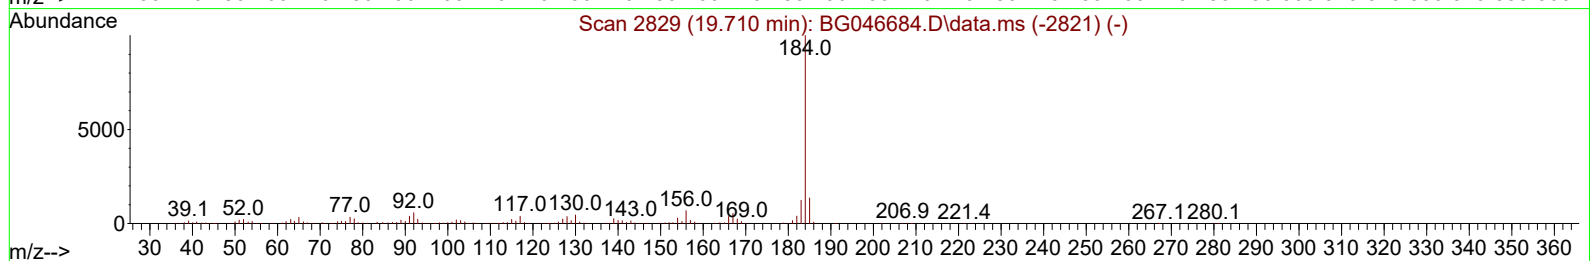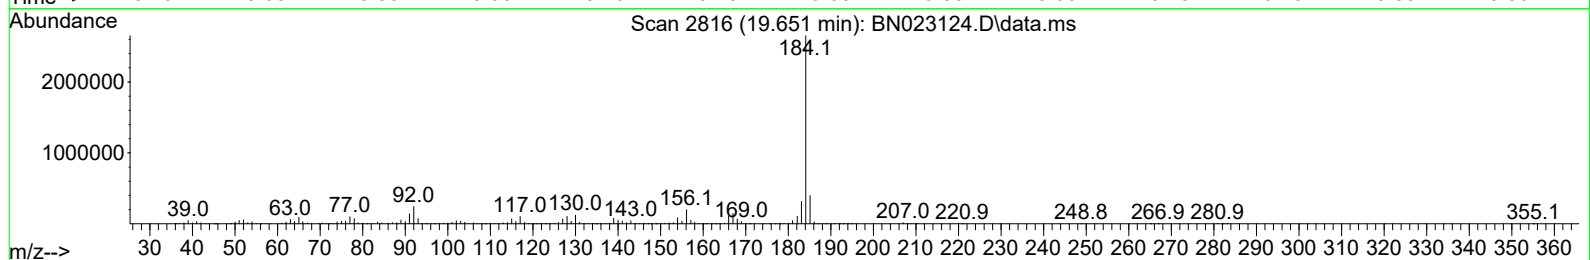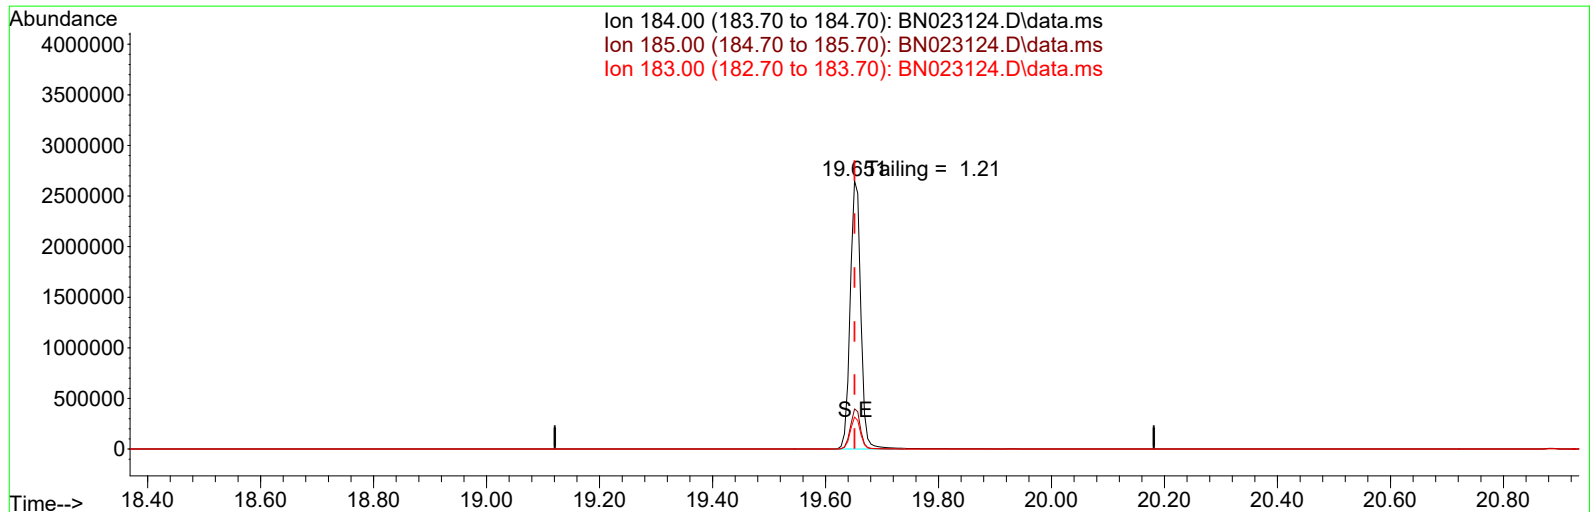

TIC: BN023124.D\data.ms

(77) Benzidine

19.651min (+ 0.000) 0.00 ng

response 3482389

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	15.00
183.00	13.20	11.94
0.00	0.00	0.00