
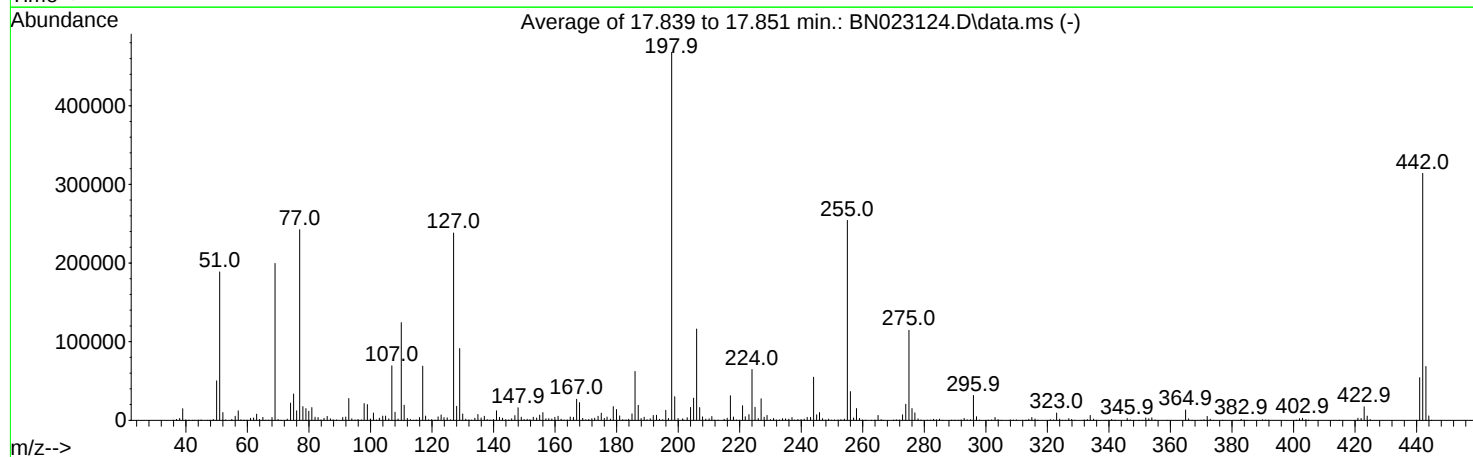


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121022\
 Data File : BN023124.D
 Acq On : 10 Dec 2022 16:34
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN120822.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Dec 12 05:18:26 2022

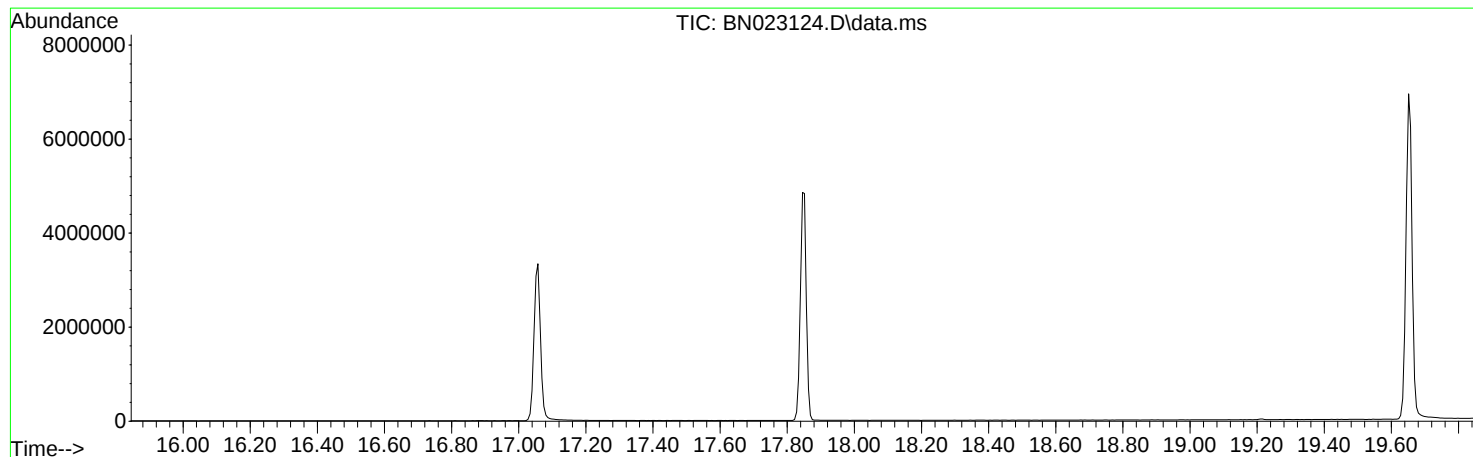




AutoFind: Scans 2508, 2509, 2510; Background Corrected with Scan 2501

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	40.3	188630	PASS
68	69	0.00	2	1.7	3478	PASS
69	198	0.00	100	42.7	199509	PASS
70	69	0.00	2	0.6	1114	PASS
127	198	10	80	50.9	238101	PASS
197	198	0.00	2	0.5	2268	PASS
198	198	100	100	100.0	467776	PASS
199	198	5	9	6.4	30125	PASS
275	198	10	60	24.5	114488	PASS
365	198	1	100	2.8	13121	PASS
441	198	0.01	100	11.6	54189	PASS
442	442	50	100	100.0	314133	PASS
443	442	15	24	21.8	68384	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121022\
Data File : BN023124.D
Acq On : 10 Dec 2022 16:34
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Dec 12 07:12:41 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 12 07:11:25 2022
Response via : Initial Calibration

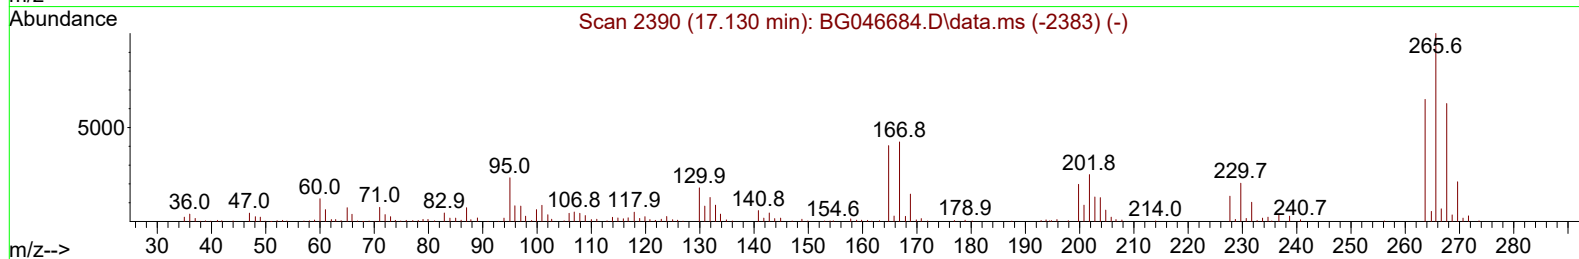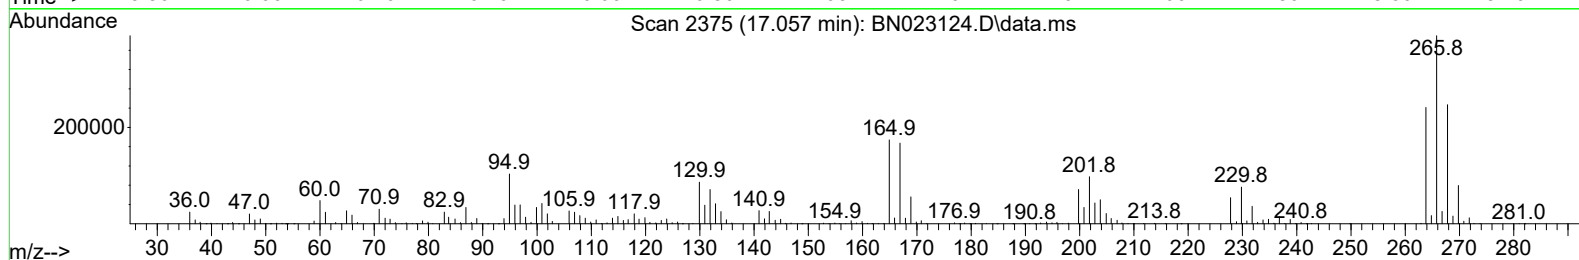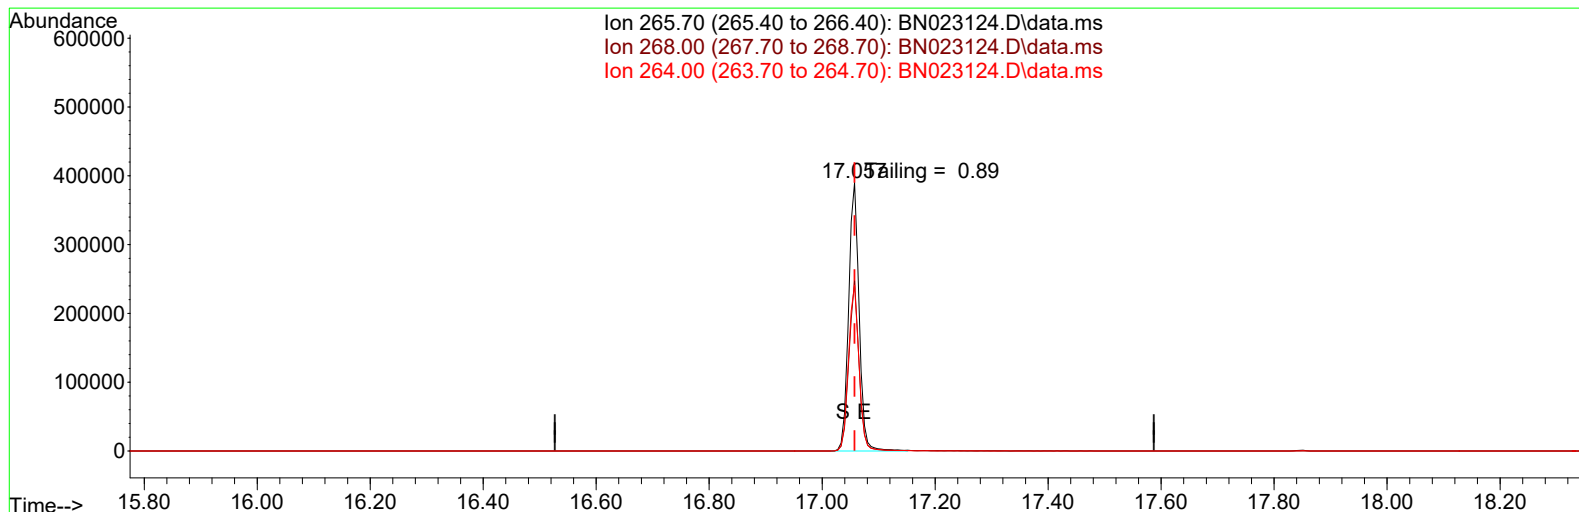

TIC: BN023124.D\data.ms

(70) Pentachlorophenol (C)

17.057min (+ 0.000) 19581.30 ng




response 505725

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	63.35
264.00	61.60	61.86
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121022\
Data File : BN023124.D
Acq On : 10 Dec 2022 16:34
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Dec 12 07:12:41 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 12 07:11:25 2022
Response via : Initial Calibration

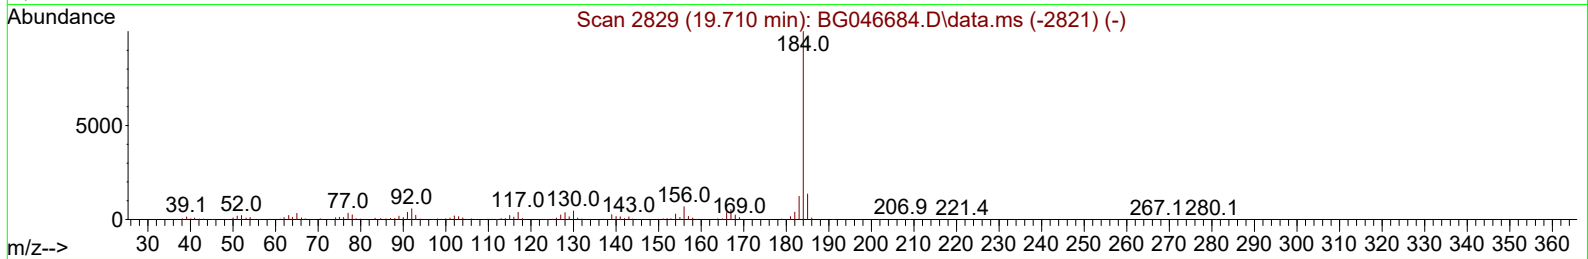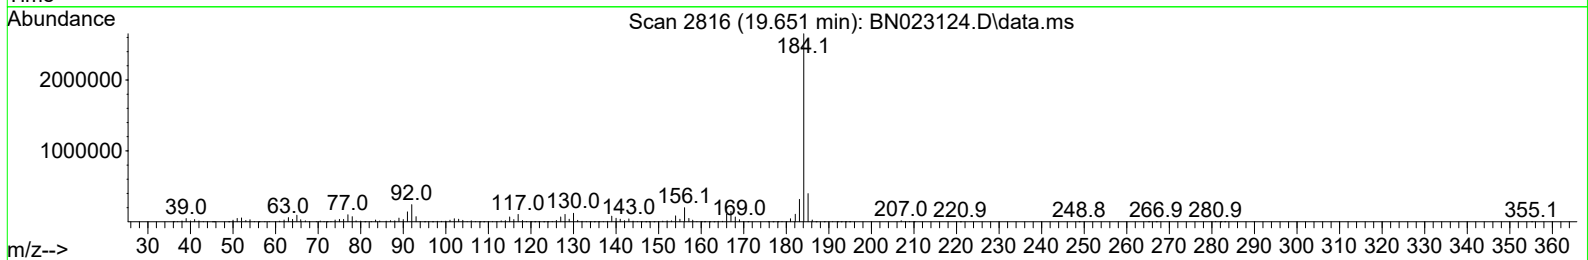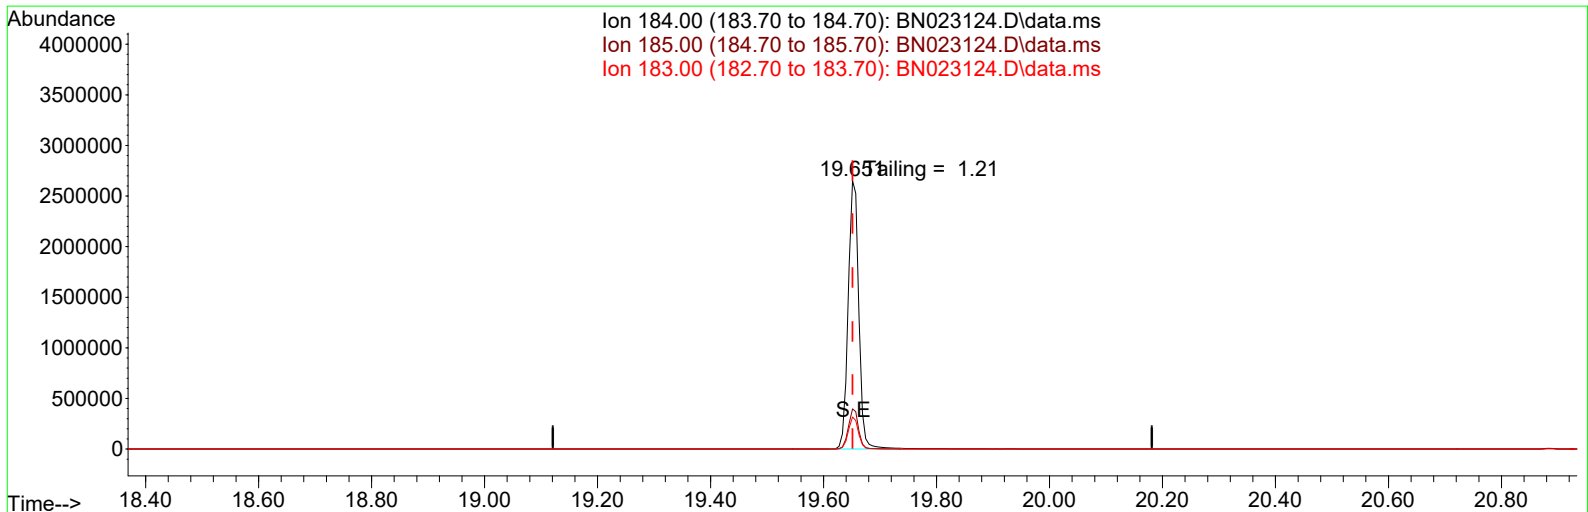

TIC: BN023124.D\data.ms

(77) Benzidine

19.651min (+ 0.000) 0.00 ng

response 3482389

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	15.00
183.00	13.20	11.94
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
12/10/2022	BNA_N	<u>BN023124.D</u>
Compound Name	Response	Retention Time
DDT	1580141	20.886
DDD	14669	20.498
DDE	261	19.933
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
14930	1595071	0.94

Instrument :
BNA_N
ClientSampleId :
DFTPP