




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121024\
Data File : BN035564.D
Acq On : 11 Dec 2024 13:40
Operator : RC/JU
Sample : P5152-02MS
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BHK72MS

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 12/12/2024
Supervised By :mohammad ahmed 12/12/2024

Quant Time: Dec 11 14:47:01 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN111624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 10 16:10:57 2024
Response via : Initial Calibration

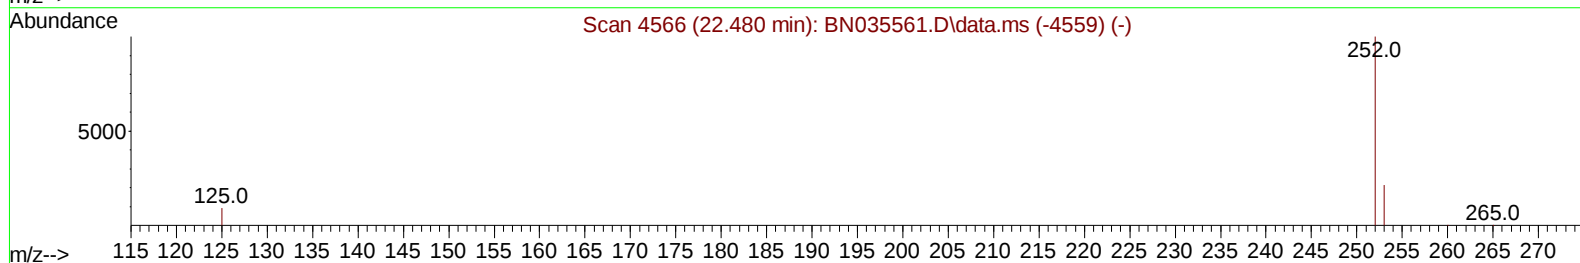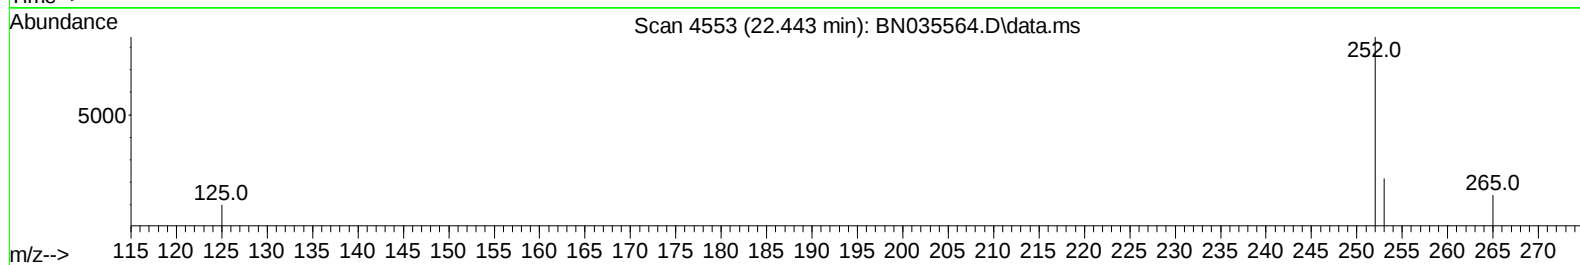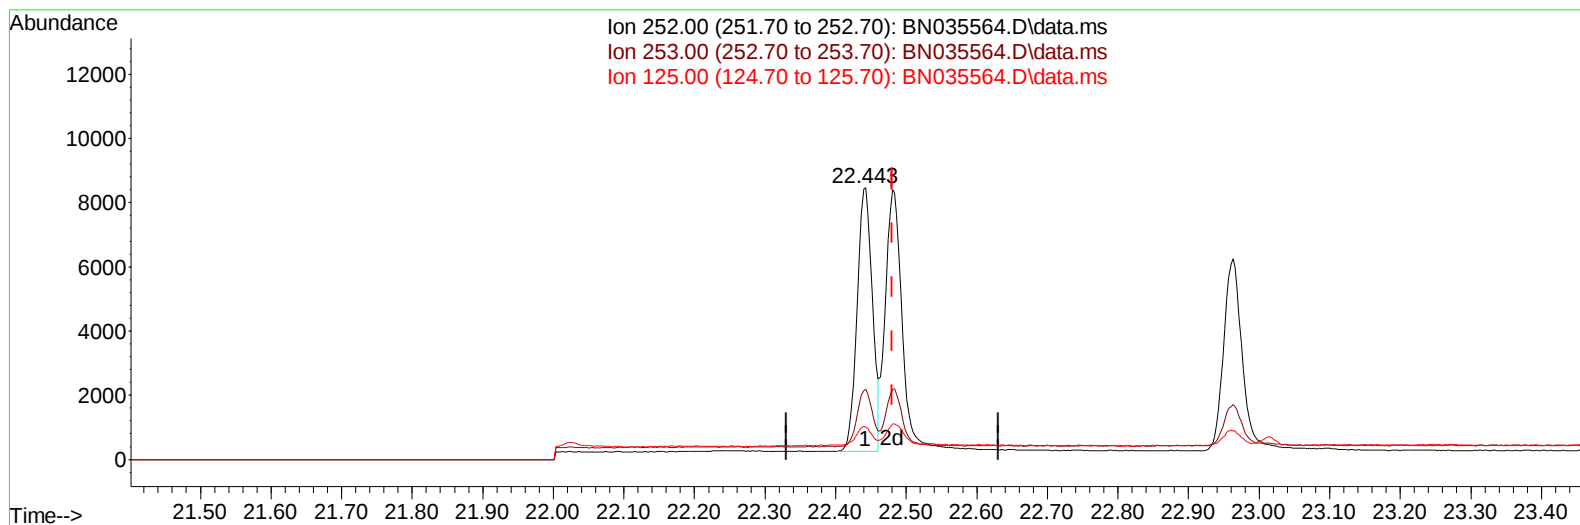

TIC: BN035564.D\data.ms

(25) Benzo(k)fluoranthene

22.443min (-0.038) 0.41 ng/u1

response 12313

Ion	Exp%	Act%
252.00	100.00	100.00
253.00	27.20	25.83
125.00	10.70	11.90
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121024\
Data File : BN035564.D
Acq On : 11 Dec 2024 13:40
Operator : RC/JU
Sample : P5152-02MS
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BHK72MS

Manual IntegrationsAPPROVED

Quant Time: Dec 11 14:47:01 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN111624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 10 16:10:57 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 12/12/2024
Supervised By :mohammad ahmed 12/12/2024

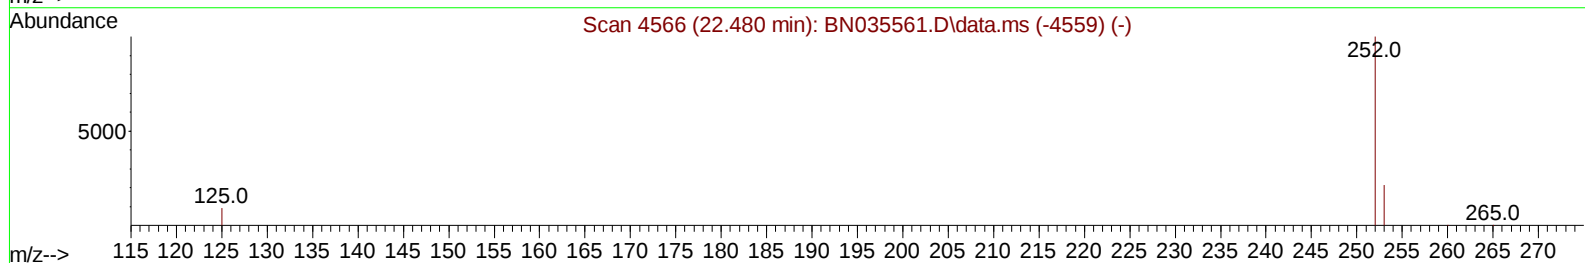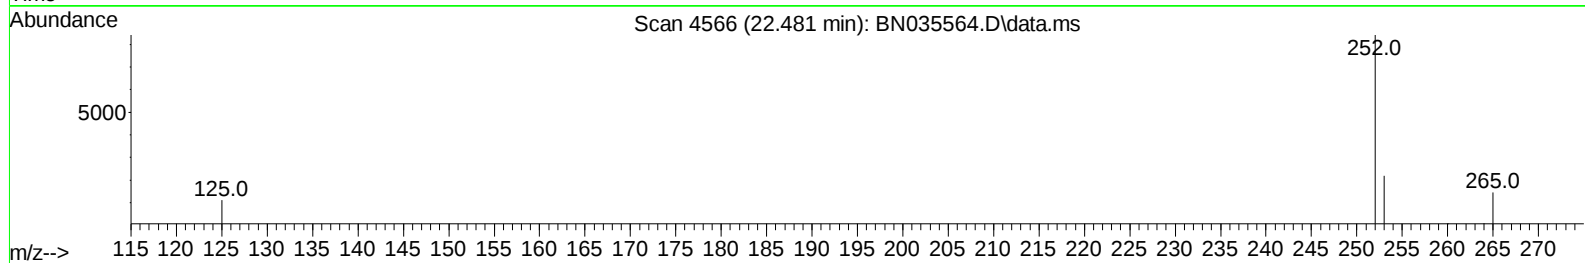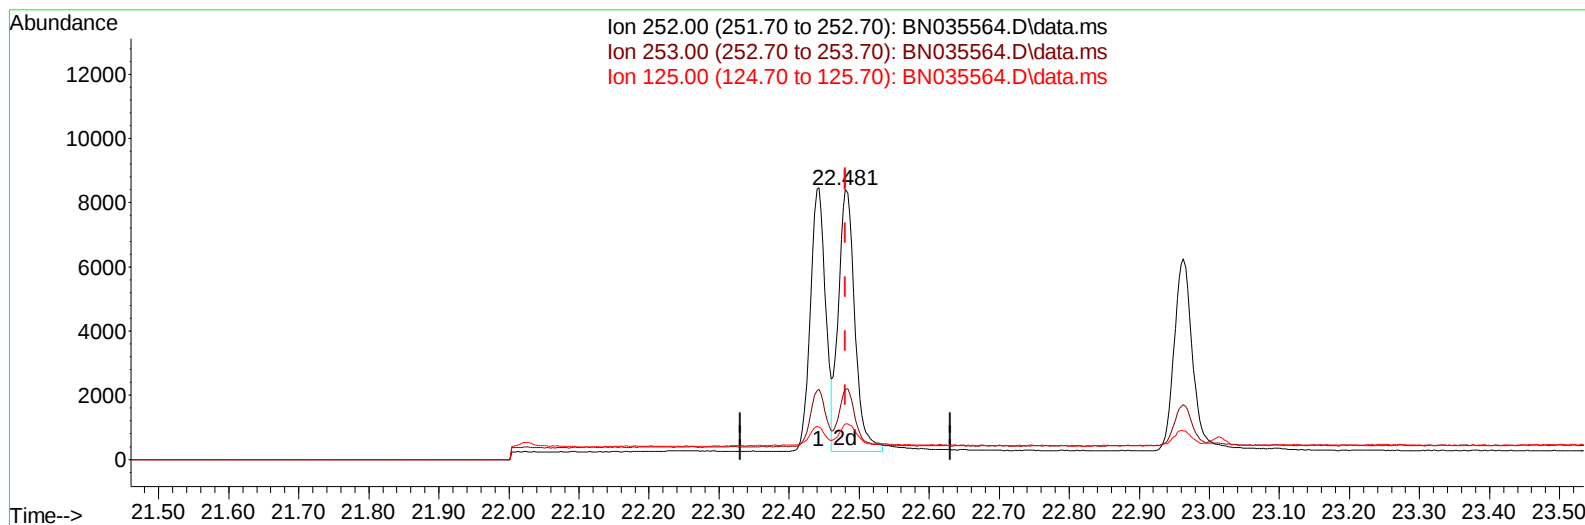

TIC: BN035564.D\data.ms

(25) Benzo(k)fluoranthene

22.481min (+ 0.000) 0.44 ng/u1 m

response 13387

Ion	Exp%	Act%
252.00	100.00	100.00
253.00	27.20	25.88
125.00	10.70	13.10#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121024\
 Data File : BN035564.D
 Acq On : 11 Dec 2024 13:40
 Operator : RC/JU
 Sample : P5152-02MS
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BHK72MS

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 12/12/2024
 Supervised By :mohammad ahmed 12/12/2024

Quant Time: Dec 11 14:47:01 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN111624.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Dec 10 16:10:57 2024
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Dichlorobenzene-d4	7.293	152		2277	0.400	ng/ul	0.00
4) Naphthalene-d8	10.036	136		6546	0.400	ng/ul	0.00
9) Acenaphthene-d10	13.949	164		4484	0.400	ng/ul	0.00
13) Phenanthrene-d10	16.717	188		9911	0.400	ng/ul	# 0.00
17) Chrysene-d12	20.964	240		8456	0.400	ng/ul	0.00
23) Perylene-d12	23.051	264		8882	0.400	ng/ul	# 0.00
System Monitoring Compounds							
3) 1,4-Dioxane-d8	2.963	96		586	0.282	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.637	152		3650	0.380	ng/ul	0.00
18) Fluoranthene-d10	18.767	212		10860	0.466	ng/ul	0.00
Target Compounds							
						Qvalue	
2) 1,4-Dioxane	2.993	88		1793	0.794	ng/ul#	83
5) Naphthalene	10.086	128		6506	0.395	ng/ul	99
7) 2-Methylnaphthalene	11.714	142		4069	0.356	ng/ul	98
8) 1-Methylnaphthalene	11.939	142		4116	0.357	ng/ul	98
10) Acenaphthylene	13.662	152		6319	0.355	ng/ul	99
11) Acenaphthene	14.014	153		4883	0.359	ng/ul	99
12) Fluorene	15.013	166		5790	0.362	ng/ul	97
14) Pentachlorophenol	16.379	266		1584	0.686	ng/ul	99
15) Phenanthrene	16.759	178		10231	0.390	ng/ul	100
16) Anthracene	16.848	178		9163	0.377	ng/ul	100
19) Fluoranthene	18.800	202		12573	0.427	ng/ul	97
20) Pyrene	19.167	202		13446	0.439	ng/ul	96
21) Benzo(a)anthracene	20.947	228		12659	0.431	ng/ul	99
22) Chrysene	20.999	228		12931	0.438	ng/ul	100
24) Benzo(b)fluoranthene	22.443	252		12313	0.419	ng/ul	97
25) Benzo(k)fluoranthene	22.481	252		13387m	0.442	ng/ul	
26) Benzo(a)pyrene	22.963	252		11205	0.418	ng/ul#	96
27) Indeno(1,2,3-cd)pyrene	25.084	276		14428	0.398	ng/ul#	98
28) Dibenzo(a,h)anthracene	25.101	278		11617	0.409	ng/ul#	95
29) Benzo(g,h,i)perylene	25.698	276		10429	0.365	ng/ul	97

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121024\
Data File : BN035564.D
Acq On : 11 Dec 2024 13:40
Operator : RC/JU
Sample : P5152-02MS
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
BHK72MS

Manual IntegrationsAPPROVED

Quant Time: Dec 11 14:47:01 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN111624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 10 16:10:57 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 12/12/2024
Supervised By :mohammad ahmed 12/12/2024

