




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121024\
Data File : BN035566.D
Acq On : 11 Dec 2024 14:52
Operator : RC/JU
Sample : P5153-01
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
E28N9

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 12/12/2024
Supervised By :mohammad ahmed 12/12/2024

Quant Time: Dec 11 15:34:20 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN111624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 10 16:10:57 2024
Response via : Initial Calibration

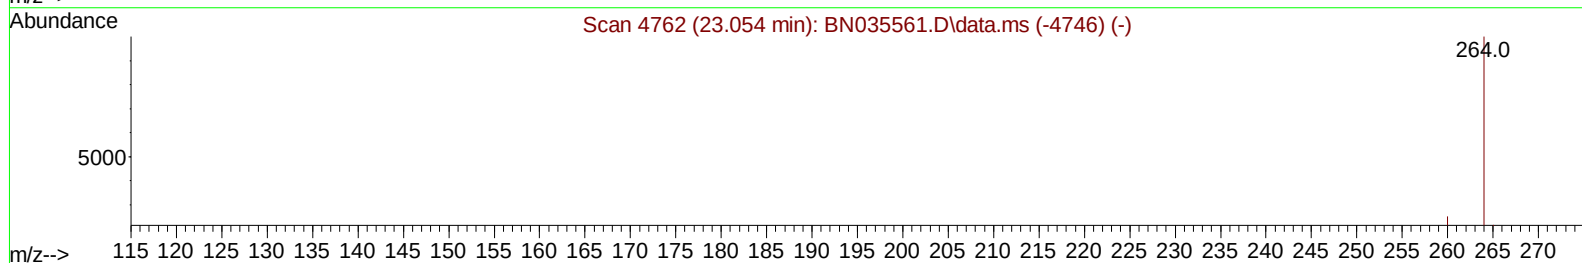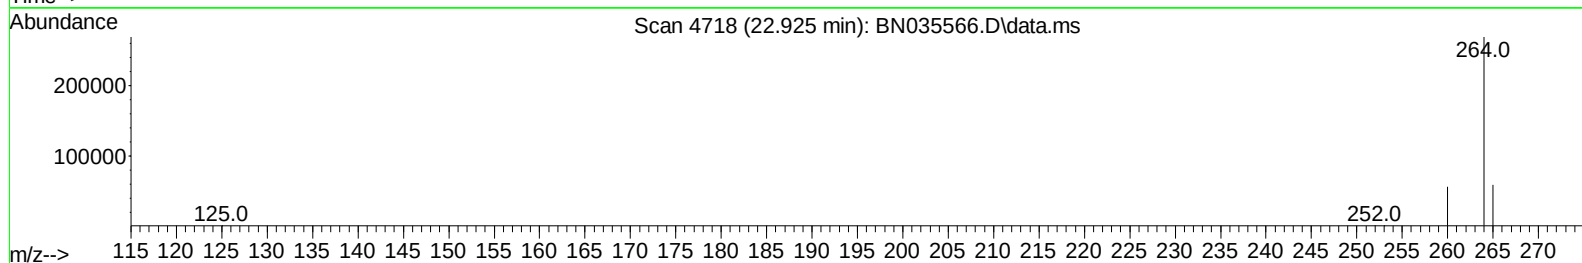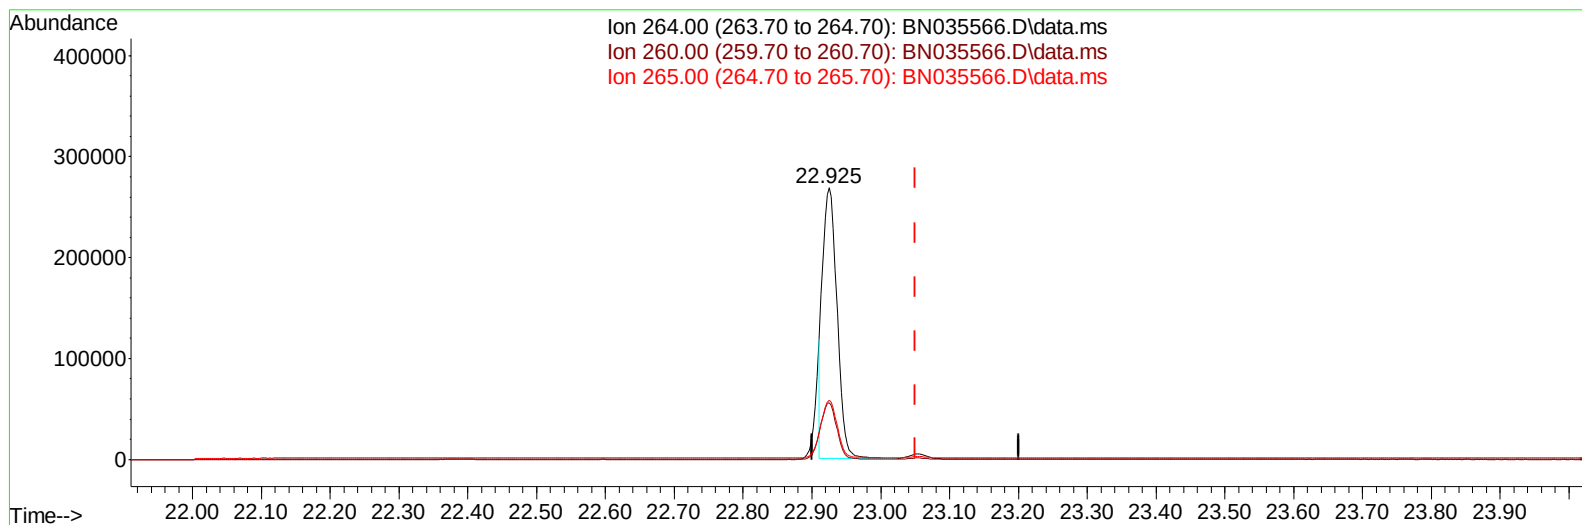

TIC: BN035566.D\data.ms

(23) Perylene-d12 (I)

22.925min (-0.125) 0.40 ng/u1

response 391206

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	26.20	20.92#
265.00	75.50	21.81#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121024\
Data File : BN035566.D
Acq On : 11 Dec 2024 14:52
Operator : RC/JU
Sample : P5153-01
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
E28N9

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 12/12/2024
Supervised By :mohammad ahmed 12/12/2024

Quant Time: Dec 11 15:34:20 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN111624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 10 16:10:57 2024
Response via : Initial Calibration

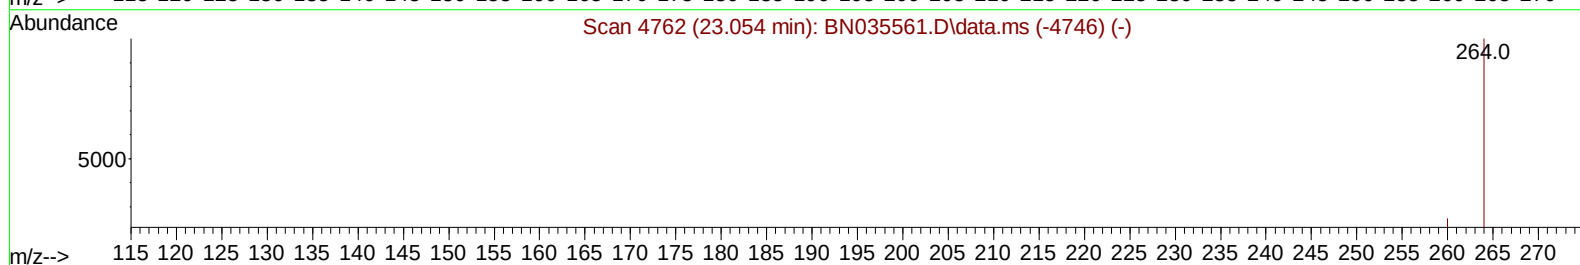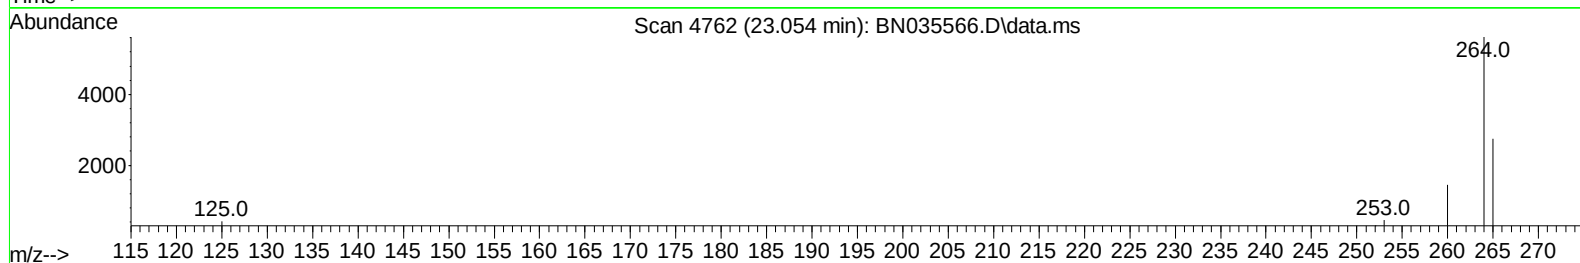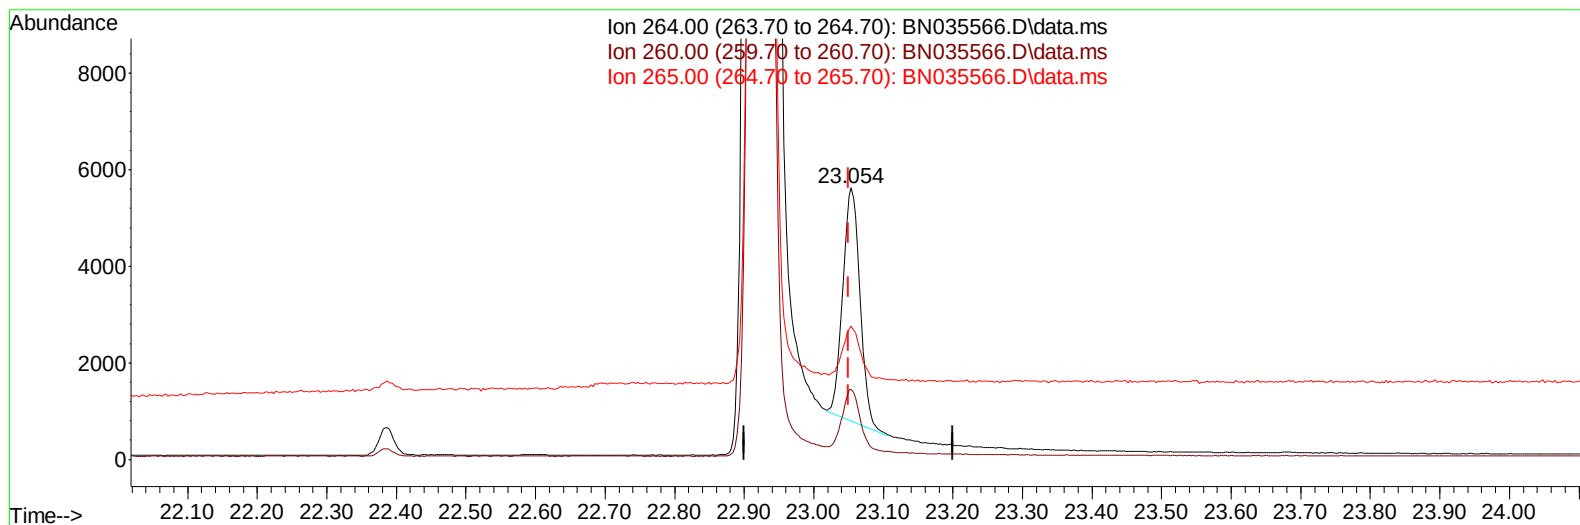

TIC: BN035566.D\data.ms

(23) Perylene-d12 (I)

23.054min (+ 0.003) 0.40 ng/ul m

response 8246

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	26.20	25.82
265.00	75.50	49.06#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121024\
 Data File : BN035566.D
 Acq On : 11 Dec 2024 14:52
 Operator : RC/JU
 Sample : P5153-01
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 E28N9

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 12/12/2024
 Supervised By :mohammad ahmed 12/12/2024

Quant Time: Dec 11 15:34:20 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN111624.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Dec 10 16:10:57 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.289	152	2523	0.400	ng/ul	0.00
4) Naphthalene-d8	10.037	136	7451	0.400	ng/ul	0.00
9) Acenaphthene-d10	13.949	164	4969	0.400	ng/ul	0.00
13) Phenanthrene-d10	16.717	188	10726	0.400	ng/ul	0.00
17) Chrysene-d12	20.964	240	8254	0.400	ng/ul	0.00
23) Perylene-d12	23.054	264	8246m	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	2.964	96	9645	4.183	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.637	152	2378	0.218	ng/ul	0.00
18) Fluoranthene-d10	18.768	212	5412	0.238	ng/ul	0.00

Target Compounds	Qvalue
------------------	--------

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121024\
Data File : BN035566.D
Acq On : 11 Dec 2024 14:52
Operator : RC/JU
Sample : P5153-01
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
E28N9

Manual IntegrationsAPPROVED

Quant Time: Dec 11 15:34:20 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN111624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 10 16:10:57 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 12/12/2024
Supervised By :mohammad ahmed 12/12/2024

