




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121024\
Data File : BN035567.D
Acq On : 11 Dec 2024 15:29
Operator : RC/JU
Sample : P5153-02
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
E28P0

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 12/12/2024
Supervised By :mohammad ahmed 12/12/2024

Quant Time: Dec 11 17:49:26 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN111624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 10 16:10:57 2024
Response via : Initial Calibration

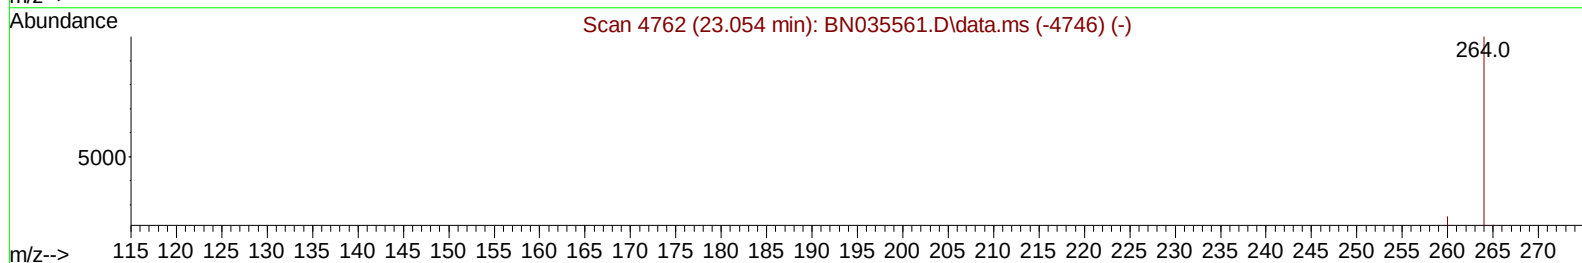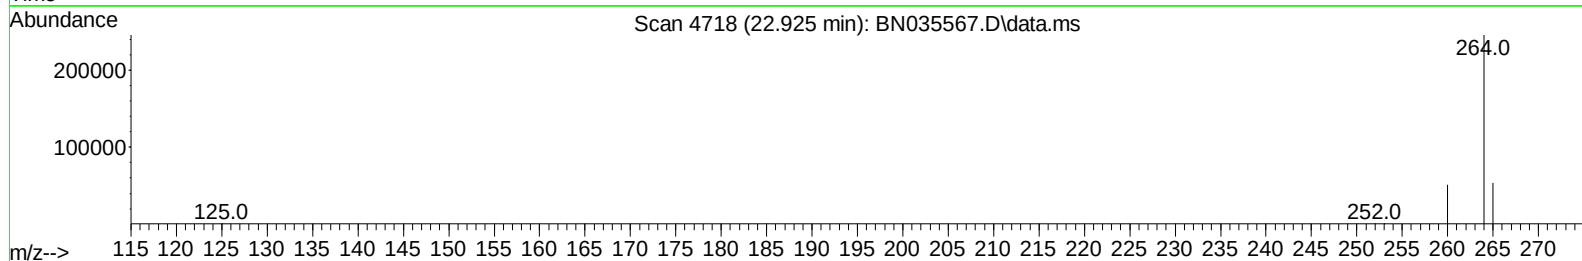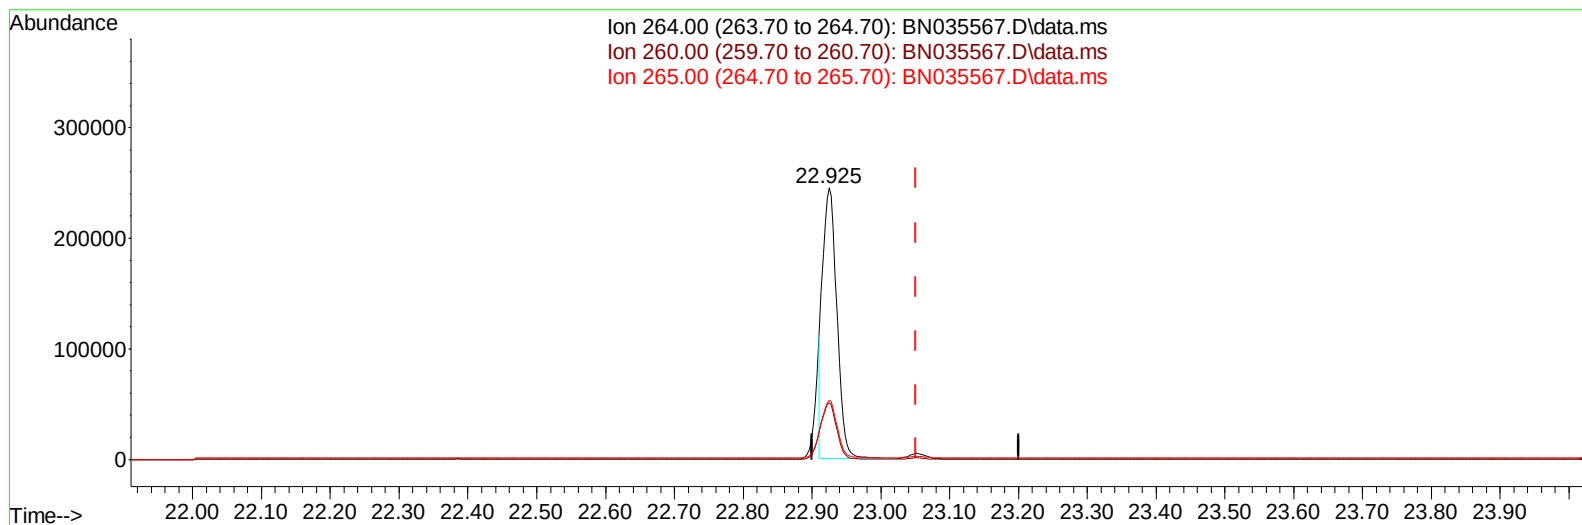

TIC: BN035567.D\data.ms

(23) Perylene-d12 (I)

22.925min (-0.126) 0.40 ng/u1

response 351360

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	26.20	20.80#
265.00	75.50	21.72#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121024\
Data File : BN035567.D
Acq On : 11 Dec 2024 15:29
Operator : RC/JU
Sample : P5153-02
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
E28P0

Manual IntegrationsAPPROVED

Quant Time: Dec 11 17:49:26 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN111624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 10 16:10:57 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 12/12/2024
Supervised By :mohammad ahmed 12/12/2024

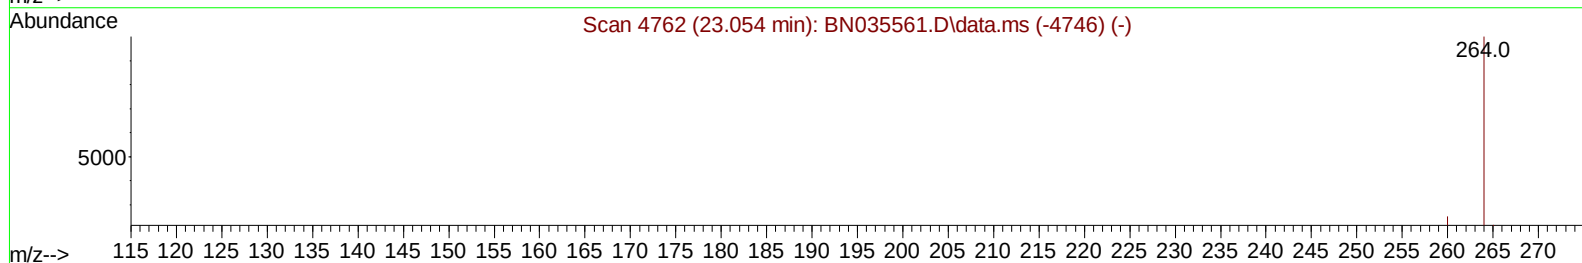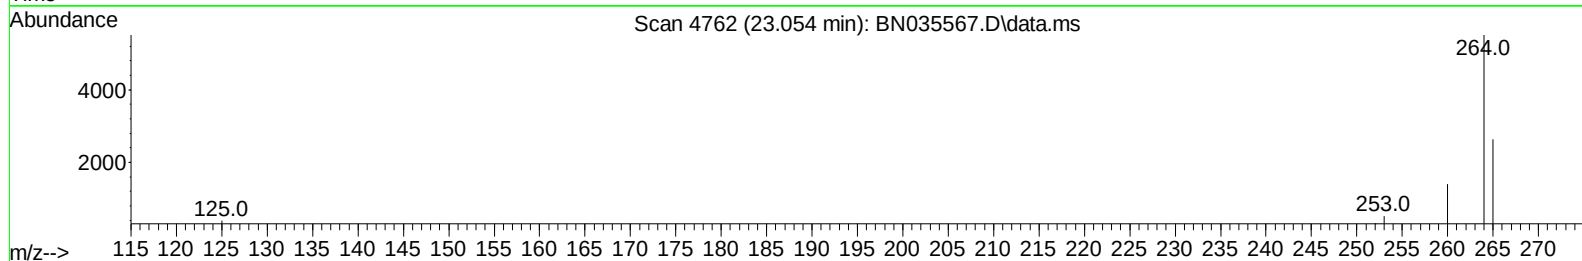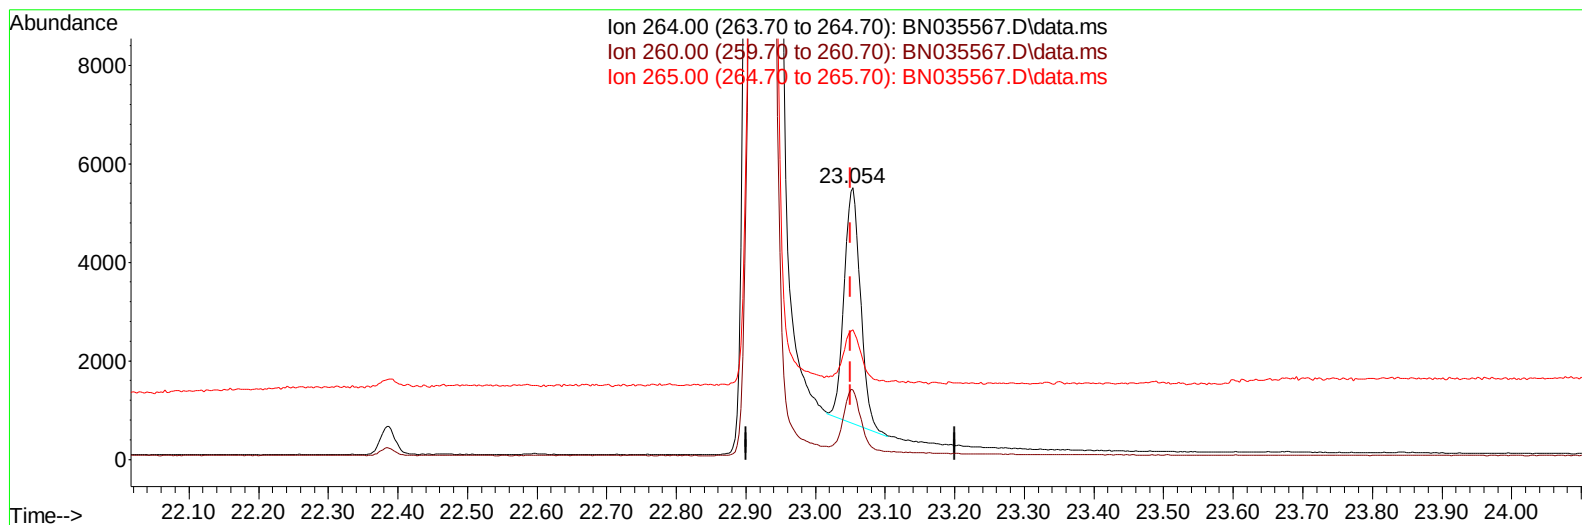

TIC: BN035567.D\data.ms

(23) Perylene-d12 (I)

23.054min (+ 0.003) 0.40 ng/ul m

response 7854

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	26.20	25.50
265.00	75.50	47.70#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121024\
 Data File : BN035567.D
 Acq On : 11 Dec 2024 15:29
 Operator : RC/JU
 Sample : P5153-02
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 E28P0

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 12/12/2024
 Supervised By :mohammad ahmed 12/12/2024

Quant Time: Dec 11 17:49:26 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN111624.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Dec 10 16:10:57 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.288	152	2704	0.400	ng/ul	0.00
4) Naphthalene-d8	10.037	136	8379	0.400	ng/ul	0.00
9) Acenaphthene-d10	13.949	164	5349	0.400	ng/ul	0.00
13) Phenanthrene-d10	16.717	188	11428	0.400	ng/ul	0.00
17) Chrysene-d12	20.964	240	8652	0.400	ng/ul	0.00
23) Perylene-d12	23.054	264	7854m	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	2.963	96	9045	3.660	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.637	152	2330	0.190	ng/ul	0.00
18) Fluoranthene-d10	18.768	212	5473	0.229	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121024\
Data File : BN035567.D
Acq On : 11 Dec 2024 15:29
Operator : RC/JU
Sample : P5153-02
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
E28P0

Manual IntegrationsAPPROVED

Quant Time: Dec 11 17:49:26 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN11624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 10 16:10:57 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 12/12/2024
Supervised By :mohammad ahmed 12/12/2024

