




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121024\
Data File : BN035576.D
Acq On : 11 Dec 2024 20:54
Operator : RC/JU
Sample : PB165482BL
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK482

Manual IntegrationsAPPROVED

Quant Time: Dec 11 22:10:32 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN111624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 10 16:10:57 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 12/12/2024
Supervised By :mohammad ahmed 12/12/2024

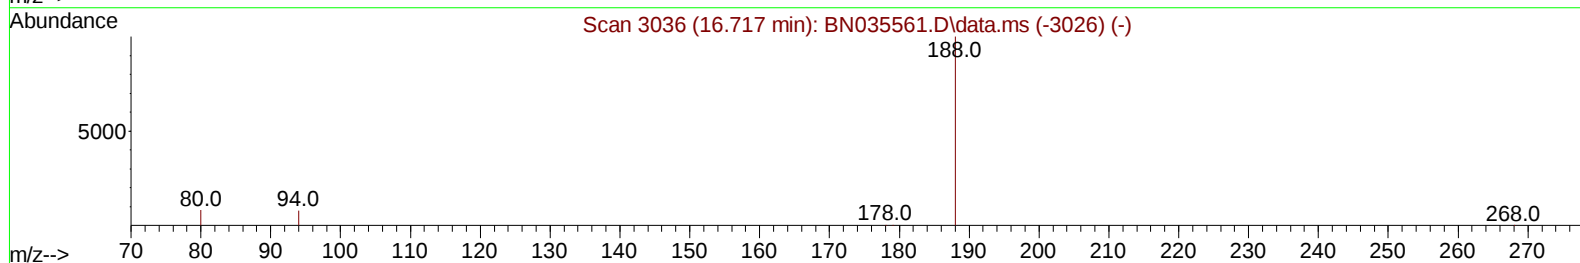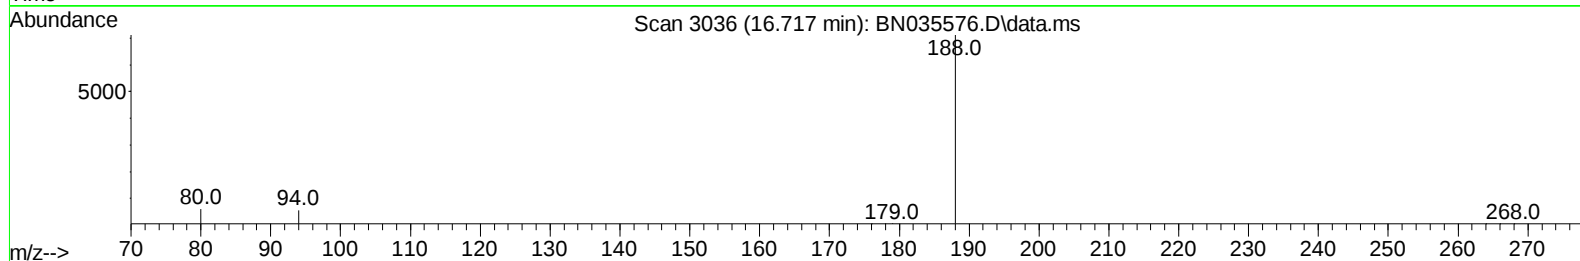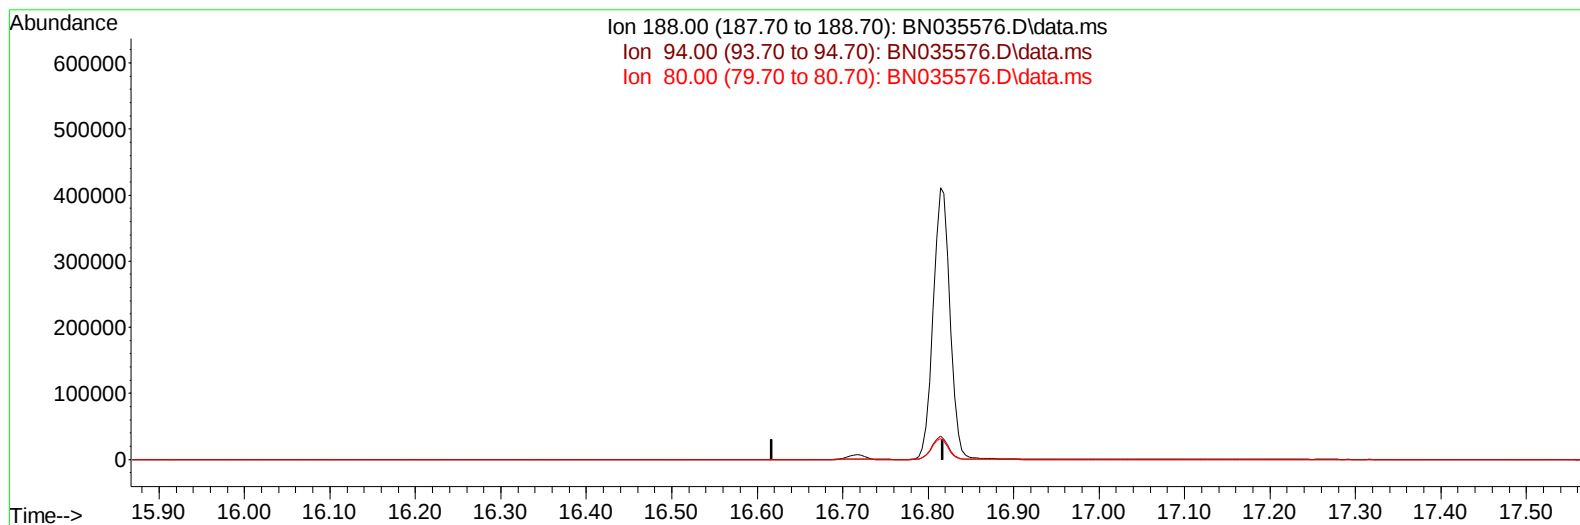

TIC: BN035576.D\data.ms

(13) Phenanthrene-d10 (I)

16.717min (-16.717) 0.00 ng/u1

response 0

Ion	Exp%	Act%
188.00	100.00	0.00
94.00	7.00	0.00#
80.00	7.60	0.00#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121024\
 Data File : BN035576.D
 Acq On : 11 Dec 2024 20:54
 Operator : RC/JU
 Sample : PB165482BL
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK482

Manual IntegrationsAPPROVED

Quant Time: Dec 11 22:10:32 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN111624.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Dec 10 16:10:57 2024
 Response via : Initial Calibration

Reviewed By :Yogesh Patel 12/12/2024
 Supervised By :mohammad ahmed 12/12/2024

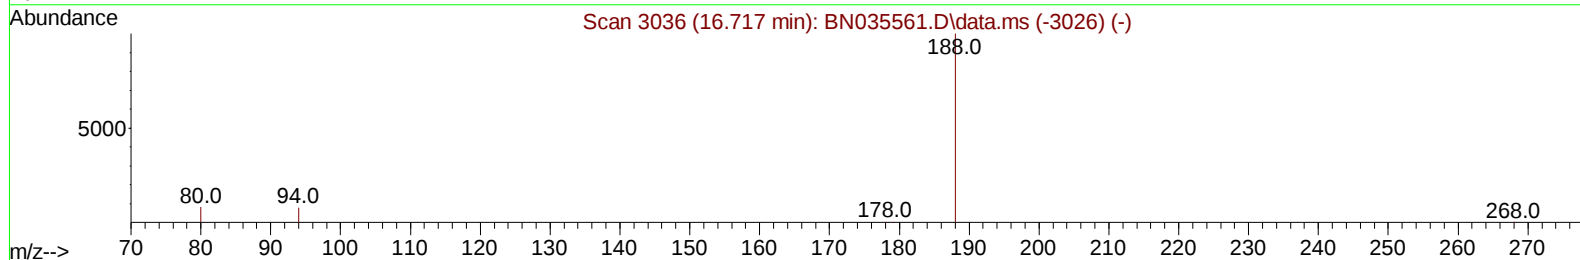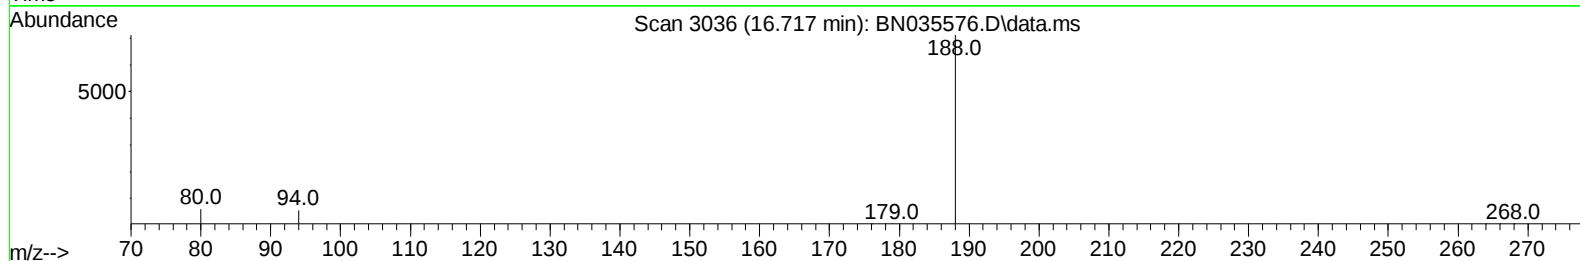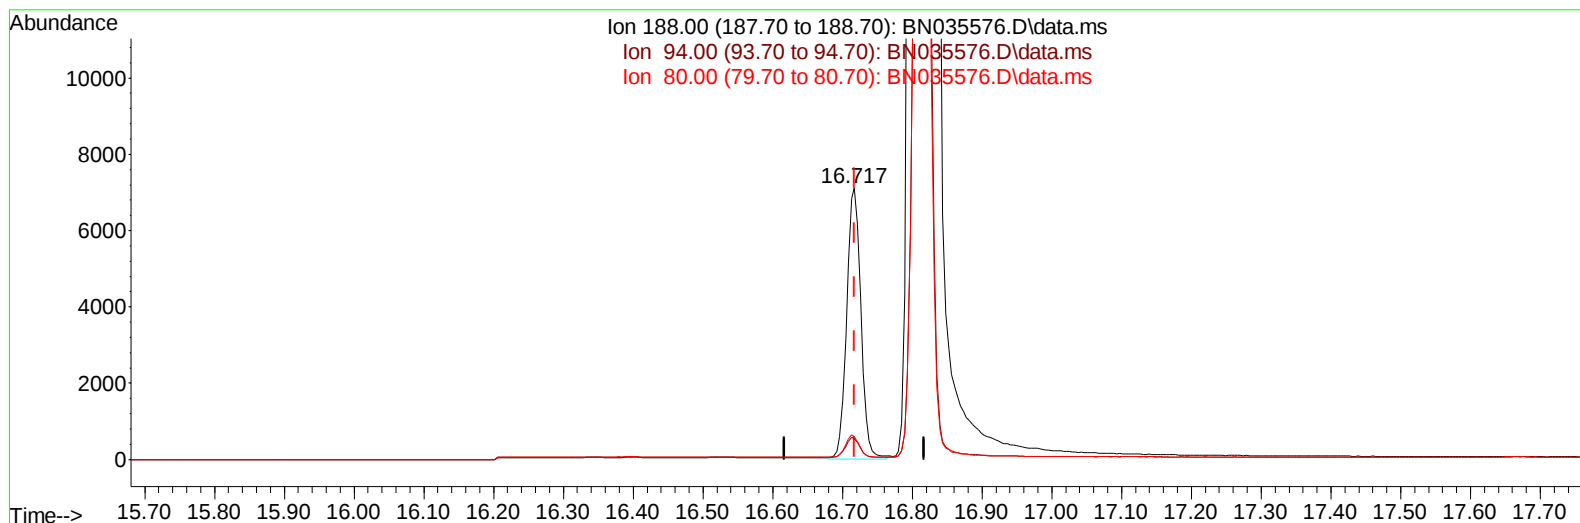

TIC: BN035576.D\data.ms

(13) Phenanthrene-d10 (I)

16.717min (-0.000) 0.40 ng/ul m

response 10004

Ion	Exp%	Act%
188.00	100.00	100.00
94.00	7.00	7.74
80.00	7.60	8.44
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121024\
Data File : BN035576.D
Acq On : 11 Dec 2024 20:54
Operator : RC/JU
Sample : PB165482BL
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK482

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 12/12/2024
Supervised By :mohammad ahmed 12/12/2024

Quant Time: Dec 11 22:10:32 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN111624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 10 16:10:57 2024
Response via : Initial Calibration

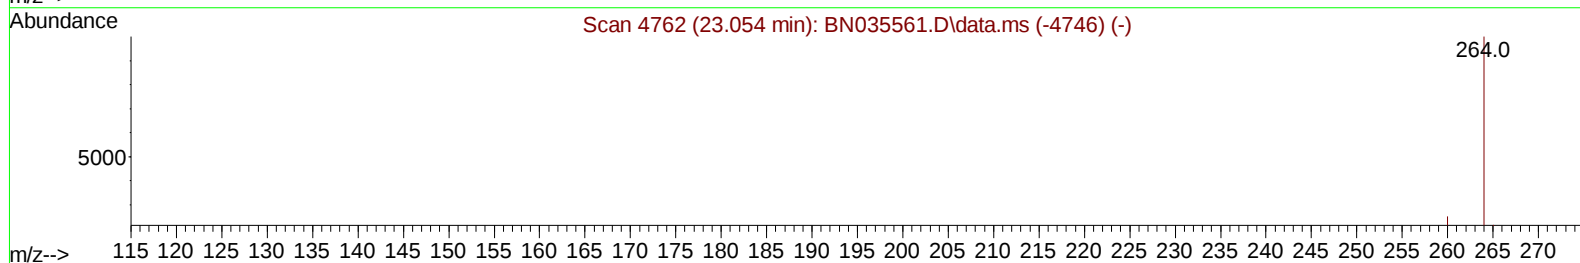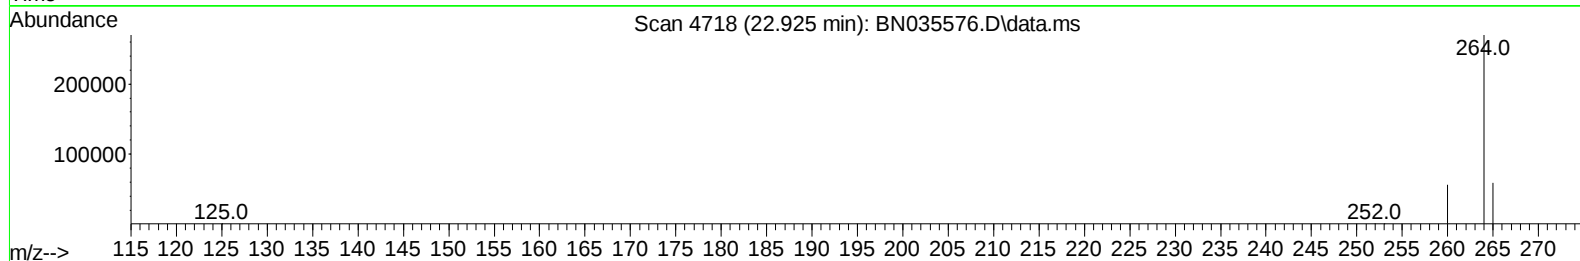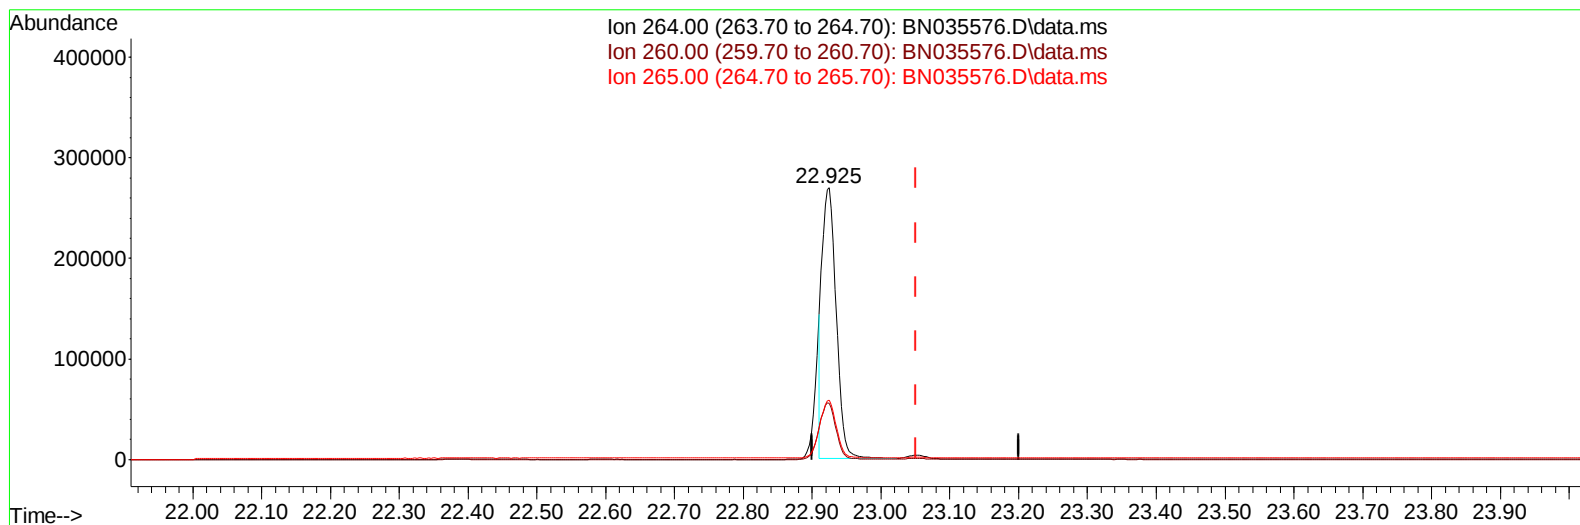

TIC: BN035576.D\data.ms

(23) Perylene-d12 (I)

22.925min (-0.126) 0.40 ng/u1

response 382297

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	26.20	20.71#
265.00	75.50	21.80#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121024\
Data File : BN035576.D
Acq On : 11 Dec 2024 20:54
Operator : RC/JU
Sample : PB165482BL
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK482

Manual IntegrationsAPPROVED

Quant Time: Dec 11 22:10:32 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN111624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 10 16:10:57 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 12/12/2024
Supervised By :mohammad ahmed 12/12/2024

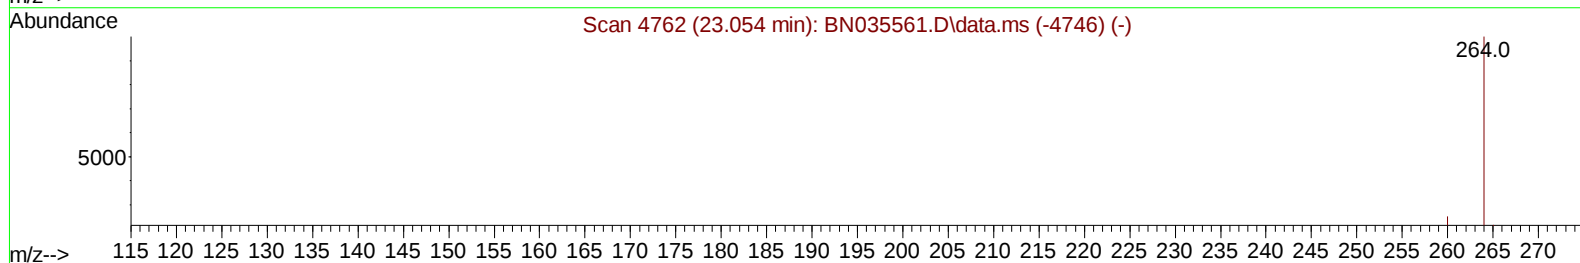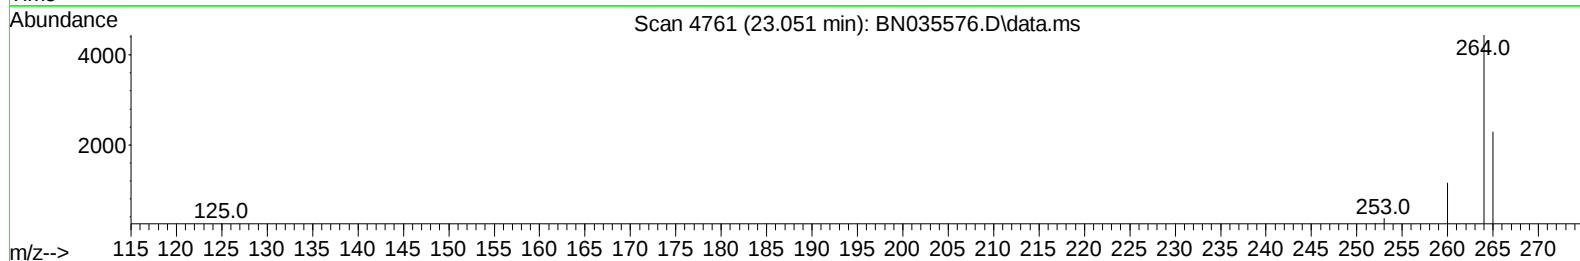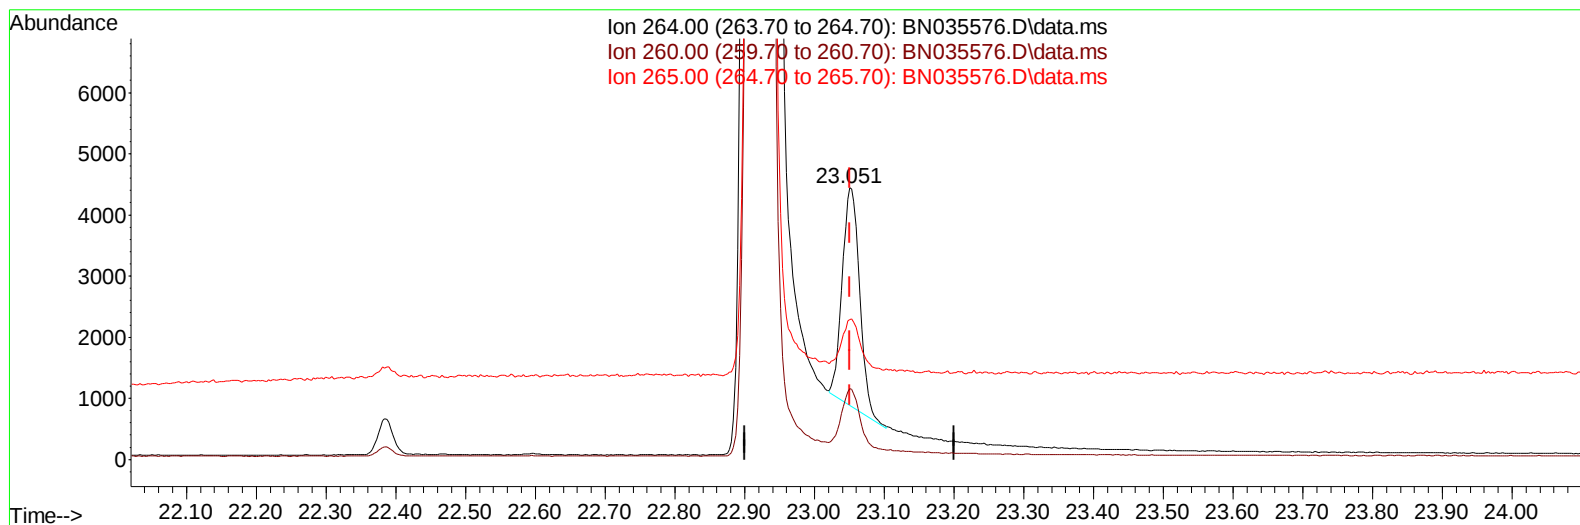

TIC: BN035576.D\data.ms

(23) Perylene-d12 (I)

23.051min (-0.000) 0.40 ng/ul m

response 6097

Ion	Exp%	Act%
264.00	100.00	100.00
260.00	26.20	26.05
265.00	75.50	51.60#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121024\
 Data File : BN035576.D
 Acq On : 11 Dec 2024 20:54
 Operator : RC/JU
 Sample : PB165482BL
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SBLK482

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 12/12/2024
 Supervised By :mohammad ahmed 12/12/2024

Quant Time: Dec 11 22:10:32 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN111624.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Dec 10 16:10:57 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.288	152	2556	0.400	ng/ul	0.00
4) Naphthalene-d8	10.036	136	7158	0.400	ng/ul	0.00
9) Acenaphthene-d10	13.949	164	4707	0.400	ng/ul	0.00
13) Phenanthrene-d10	16.717	188	10004m	0.400	ng/ul	0.00
17) Chrysene-d12	20.964	240	6679	0.400	ng/ul	0.00
23) Perylene-d12	23.051	264	6097m	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	2.959	96	13037	5.581	ng/ul	0.00
6) 2-Methylnaphthalene-d10	11.642	152	2673	0.255	ng/ul	0.00
18) Fluoranthene-d10	18.767	212	5597	0.304	ng/ul	0.00

Target Compounds	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121024\
Data File : BN035576.D
Acq On : 11 Dec 2024 20:54
Operator : RC/JU
Sample : PB165482BL
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SBLK482

Manual IntegrationsAPPROVED

Quant Time: Dec 11 22:10:32 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN111624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 10 16:10:57 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 12/12/2024
Supervised By :mohammad ahmed 12/12/2024

