

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121024\
 Data File : BN035563.D
 Acq On : 11 Dec 2024 13:04
 Operator : RC/JU
 Sample : P5152-01
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 BHK72

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 12/12/2024
 Supervised By :mohammad ahmed 12/12/2024

Quant Time: Dec 11 13:35:37 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN111624.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Dec 10 16:10:57 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.289	152	2833	0.400	ng/u1	0.00
4) Naphthalene-d8	10.037	136	8187	0.400	ng/u1	0.00
9) Acenaphthene-d10	13.949	164	5484	0.400	ng/u1	0.00
13) Phenanthrene-d10	16.717	188	11778m	0.400	ng/u1	0.00
17) Chrysene-d12	20.964	240	8753	0.400	ng/u1	# 0.00
23) Perylene-d12	23.051	264	8318m	0.400	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	2.963	96	11164	4.312	ng/u1	0.00
6) 2-Methylnaphthalene-d10	11.637	152	3393	0.283	ng/u1	0.00
18) Fluoranthene-d10	18.768	212	9385	0.389	ng/u1	0.00
Target Compounds						Qvalue
5) Naphthalene	10.086	128	1075m	0.052	ng/u1	

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121024\
Data File : BN035563.D
Acq On : 11 Dec 2024 13:04
Operator : RC/JU
Sample : P5152-01
Misc :
ALS Vial : 4 Sample Multiplier: 1


Instrument :
BNA_N
ClientSampleId :
BHK72

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 12/12/2024
Supervised By :mohammad ahmed 12/12/2024


Quant Time: Dec 11 13:35:37 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\SFAM-EPA-SIM-BN111624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Dec 10 16:10:57 2024
Response via : Initial Calibration

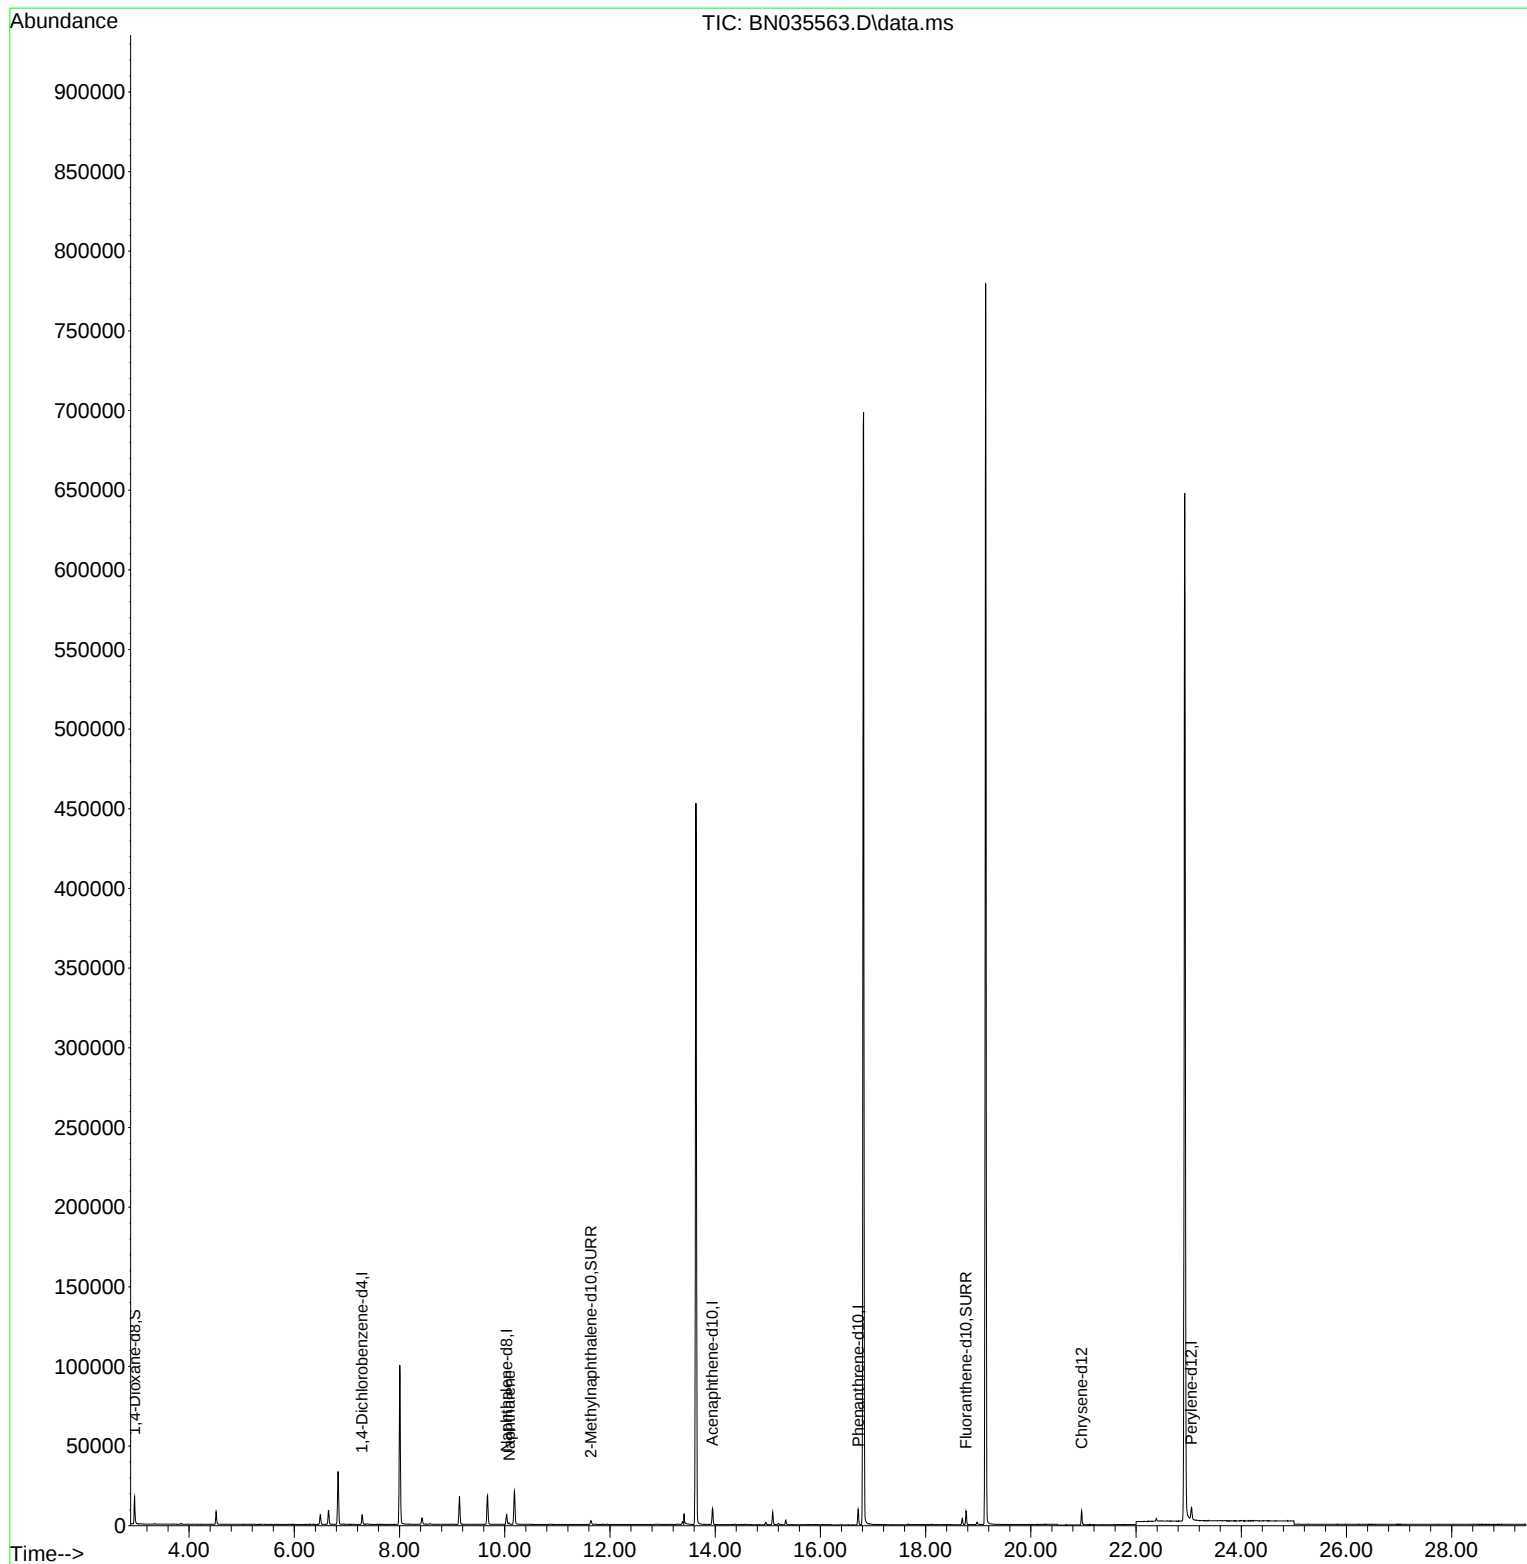

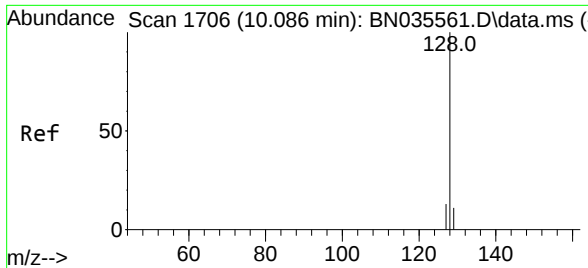

#5
Naphthalene
Concen: 0.052 ng/ul m
RT: 10.086 min Scan# 1
Delta R.T. 0.000 min
Lab File: BN035563.D
Acq: 11 Dec 2024 13:04

Instrument :
BNA_N
ClientSampleId :
BHK72

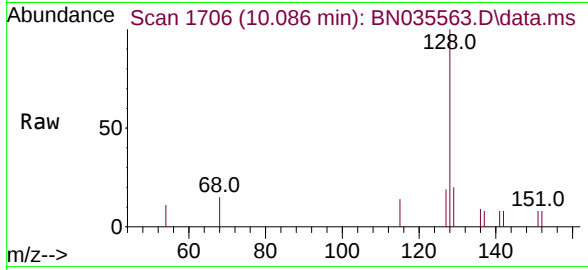

Tgt Ion:128	Resp:	1079
Ion Ratio	Lower	Upper
128	100	
129	19.9	9.9 14.9
127	19.2	11.4 17.2

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 12/12/2024
Supervised By :mohammad ahmed 12/12/2024

