

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121120\
 Data File : BN013063.D
 Acq On : 11 Dec 2020 11:45
 Operator : CG/JU
 Sample : SSTDCCC0.4
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 SSTDCCC0.4

Quant Time: Dec 11 12:49:42 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN121020.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Dec 11 01:53:51 2020
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.370	152	589	0.40	ng	0.00
7) Naphthalene-d8	10.137	136	2039	0.40	ng	# 0.00
13) Acenaphthene-d10	14.029	164	1202	0.40	ng	0.00
19) Phenanthrene-d10	16.799	188	2601	0.40	ng	# 0.00
29) Chrysene-d12	21.024	240	2746	0.40	ng	# 0.01
36) Perylene-d12	23.117	264	2981	0.40	ng	# 0.00
System Monitoring Compounds						
4) 2-Fluorophenol	4.994	112	886	0.42	ng	0.00
5) Phenol-d6	6.573	99	986	0.41	ng	0.00
8) Nitrobenzene-d5	8.540	82	816	0.38	ng	0.01
11) 2-Methylnaphthalene-d10	11.746	152	1421	0.39	ng	0.00
14) 2,4,6-Tribromophenol	15.551	330	278	0.35	ng	0.00
15) 2-Fluorobiphenyl	12.646	172	2097	0.40	ng	0.00
27) Fluoranthene-d10	18.843	212	3320	0.38	ng	0.00
31) Terphenyl-d14	19.463	244	2715	0.40	ng	0.00
Target Compounds						
						Qvalue
2) 1,4-Dioxane	2.965	88	609	0.47	ng	86
3) n-Nitrosodimethylamine	3.295	42	792	0.51	ng	# 74
6) bis(2-Chloroethyl)ether	6.822	93	696	0.43	ng	95
9) Naphthalene	10.188	128	2455	0.39	ng	# 94
10) Hexachlorobutadiene	10.454	225	577	0.43	ng	# 99
12) 2-Methylnaphthalene	11.822	142	1614	0.38	ng	93
16) Acenaphthylene	13.750	152	2413	0.38	ng	100
17) Acenaphthene	14.092	154	1607	0.40	ng	92
18) Fluorene	15.095	166	2123	0.39	ng	98
20) 4,6-Dinitro-2-methylph...	15.234	198	199	0.40	ng	# 1
21) 4-Bromophenyl-phenylether	16.008	248	507	0.84	ng	90
22) Hexachlorobenzene	16.105	284	767	0.40	ng	98
23) Atrazine	16.288	200	588	0.38	ng	# 91
24) Pentachlorophenol	16.471	266	282	0.35	ng	98
25) Phenanthrene	16.836	178	3272	0.38	ng	98
26) Anthracene	16.933	178	2819	0.37	ng	99
28) Fluoranthene	18.873	202	3967	0.38	ng	99
30) Pyrene	19.240	202	4068	0.39	ng	99
32) Benzo(a)anthracene	21.003	228	3748	0.37	ng	98
33) Chrysene	21.056	228	4174	0.40	ng	99
34) Bis(2-ethylhexyl)phtha...	20.950	149	1851	0.30	ng	97
35) Indeno(1,2,3-cd)pyrene	25.167	276	5433	0.39	ng	97
37) Benzo(b)fluoranthene	22.501	252	4366	0.39	ng	# 91
38) Benzo(k)fluoranthene	22.542	252	4737	0.40	ng	# 89
39) Benzo(a)pyrene	23.028	252	4228	0.39	ng	# 86
40) Dibenzo(a,h)anthracene	25.188	278	4645	0.39	ng	# 90
41) Benzo(g,h,i)perylene	25.790	276	5085	0.41	ng	# 94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121120\
Data File : BN013063.D
Acq On : 11 Dec 2020 11:45
Operator : CG/JU
Sample : SSTDCCC0.4
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4

Quant Time: Dec 11 12:49:42 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN121020.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 11 01:53:51 2020
Response via : Initial Calibration









#1
 1,4-Dichlorobenzene-d4
 Concen: 0.40 ng
 RT: 7.370 min Scan# 570
 Delta R.T. 0.000 min
 Lab File: BN013063.D
 Acq: 11 Dec 2020 11:45




Instrument :
 BNA_N
 ClientSampleId :
 SSTDCCC0.4


Tgt Ion: 152 Resp: 589
 Ion Ratio Lower Upper
 152 100
 150 152.9 116.6 174.8
 115 76.6 52.9 79.3



#2
 1,4-Dioxane
 Concen: 0.47 ng
 RT: 2.965 min Scan# 23
 Delta R.T. 0.008 min
 Lab File: BN013063.D
 Acq: 11 Dec 2020 11:45

Tgt Ion: 88 Resp: 609
 Ion Ratio Lower Upper
 88 100
 58 59.4 59.4 89.2
 43 36.3 32.3 48.5









#3
n-Nitrosodimethylamine
Concen: 0.51 ng
RT: 3.295 min Scan# 64
Delta R.T. -0.000 min
Lab File: BN013063.D
Acq: 11 Dec 2020 11:45




Instrument :
BNA_N
ClientSampled :
SSTDCCC0.4


Tgt Ion: 42 Resp: 792
Ion Ratio Lower Upper
42 100
74 77.9 64.4 96.6
44 183.3 2.8 4.2#



#4
2-Fluorophenol
Concen: 0.42 ng
RT: 4.994 min Scan# 275
Delta R.T. 0.008 min
Lab File: BN013063.D
Acq: 11 Dec 2020 11:45

Tgt Ion: 112 Resp: 886
Ion Ratio Lower Upper
112 100
64 65.3 49.5 74.3
63 39.5 32.0 48.0









#5
Phenol-d6
Concen: 0.41 ng
RT: 6.573 min Scan# 471
Delta R.T. -0.000 min
Lab File: BN013063.D
Acq: 11 Dec 2020 11:45




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4


Tgt Ion:	99	Resp:	986
Ion	Ratio	Lower	Upper
99	100		
42	27.3	22.4	33.6
71	43.1	37.8	56.6



#6
bis(2-Chloroethyl)ether
Concen: 0.43 ng
RT: 6.822 min Scan# 502
Delta R.T. -0.000 min
Lab File: BN013063.D
Acq: 11 Dec 2020 11:45

Tgt Ion:	93	Resp:	696
Ion	Ratio	Lower	Upper
93	100		
63	75.0	63.1	94.7
95	29.9	26.1	39.1









#7
Naphthalene-d8
Concen: 0.40 ng
RT: 10.137 min Scan# 831
Delta R.T. -0.000 min
Lab File: BN013063.D
Acq: 11 Dec 2020 11:45




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4


Tgt Ion:	136	Resp:	2039
Ion	Ratio	Lower	Upper
136	100		
137	15.6	10.6	15.8
54	12.3	8.6	12.8
68	9.4	5.7	8.5#



#8
Nitrobenzene-d5
Concen: 0.38 ng
RT: 8.540 min Scan# 705
Delta R.T. 0.012 min
Lab File: BN013063.D
Acq: 11 Dec 2020 11:45

Tgt Ion:	82	Resp:	816
Ion	Ratio	Lower	Upper
82	100		
128	50.4	30.6	46.0#
54	63.4	48.3	72.5









#9
Naphthalene
Concen: 0.39 ng
RT: 10.188 min Scan# 835
Delta R.T. -0.000 min
Lab File: BN013063.D
Acq: 11 Dec 2020 11:45




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4


Tgt Ion:128 Resp: 2455
Ion Ratio Lower Upper
128 100
129 15.3 9.8 14.8#
127 17.3 12.2 18.4



#10
Hexachlorobutadiene
Concen: 0.43 ng
RT: 10.454 min Scan# 856
Delta R.T. -0.013 min
Lab File: BN013063.D
Acq: 11 Dec 2020 11:45

Tgt Ion:225 Resp: 577
Ion Ratio Lower Upper
225 100
223 0.0 0.0 0.0
227 62.7 51.0 76.6









#11
2-Methylnaphthalene-d10
Concen: 0.39 ng
RT: 11.746 min Scan# 993
Delta R.T. 0.004 min
Lab File: BN013063.D
Acq: 11 Dec 2020 11:45




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4


Tgt Ion:152 Resp: 1421
Ion Ratio Lower Upper
152 100
151 19.1 16.7 25.1



#12
2-Methylnaphthalene
Concen: 0.38 ng
RT: 11.822 min Scan# 1010
Delta R.T. 0.004 min
Lab File: BN013063.D
Acq: 11 Dec 2020 11:45

Tgt Ion:142 Resp: 1614
Ion Ratio Lower Upper
142 100
141 90.8 69.4 104.2
115 52.4 35.7 53.5









#13
Acenaphthene-d10
Concen: 0.40 ng
RT: 14.029 min Scan# 1284
Delta R.T. -0.000 min
Lab File: BN013063.D
Acq: 11 Dec 2020 11:45




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4


Tgt Ion:	164	Resp:	1202
Ion	Ratio	Lower	Upper
164	100		
162	103.3	80.6	120.8
160	50.9	39.5	59.3



#14
2,4,6-Tribromophenol
Concen: 0.35 ng
RT: 15.551 min Scan# 1404
Delta R.T. -0.000 min
Lab File: BN013063.D
Acq: 11 Dec 2020 11:45

Tgt Ion:	330	Resp:	278
Ion	Ratio	Lower	Upper
330	100		
332	0.0	0.0	0.0
141	43.5	34.4	51.6









#15
2-Fluorobiphenyl
Concen: 0.40 ng
RT: 12.646 min Scan# 1175
Delta R.T. -0.000 min
Lab File: BN013063.D
Acq: 11 Dec 2020 11:45




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4


Tgt Ion:	172	Resp:	2097
Ion	Ratio	Lower	Upper
172	100		
171	37.8	28.2	42.4
170	27.0	20.0	30.0



#16
Acenaphthylene
Concen: 0.38 ng
RT: 13.750 min Scan# 1262
Delta R.T. -0.000 min
Lab File: BN013063.D
Acq: 11 Dec 2020 11:45

Tgt Ion:	152	Resp:	2413
Ion	Ratio	Lower	Upper
152	100		
151	19.8	15.8	23.8
153	13.6	10.6	16.0









#17
Acenaphthene
Concen: 0.40 ng
RT: 14.092 min Scan# 1289
Delta R.T. -0.000 min
Lab File: BN013063.D
Acq: 11 Dec 2020 11:45




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4


Tgt Ion:154 Resp: 1607
Ion Ratio Lower Upper
154 100
153 116.0 83.6 125.4
152 56.6 43.9 65.9



#18
Fluorene
Concen: 0.39 ng
RT: 15.095 min Scan# 1368
Delta R.T. -0.000 min
Lab File: BN013063.D
Acq: 11 Dec 2020 11:45

Tgt Ion:166 Resp: 2123
Ion Ratio Lower Upper
166 100
165 96.2 78.6 118.0
167 14.1 10.7 16.1









#19
Phenanthrene-d10
Concen: 0.40 ng
RT: 16.799 min Scan# 1505
Delta R.T. -0.000 min
Lab File: BN013063.D
Acq: 11 Dec 2020 11:45




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4


Tgt Ion:188	Resp:	2601
Ion Ratio	Lower	Upper
188	100	
94	0.0	0.0
80	9.5	5.0



#20
4,6-Dinitro-2-methylphenol
Concen: 0.40 ng
RT: 15.234 min Scan# 1379
Delta R.T. 0.000 min
Lab File: BN013063.D
Acq: 11 Dec 2020 11:45

Tgt Ion:198	Resp:	199
Ion Ratio	Lower	Upper
198	100	
51	132.6	43.5
105	82.6	27.2







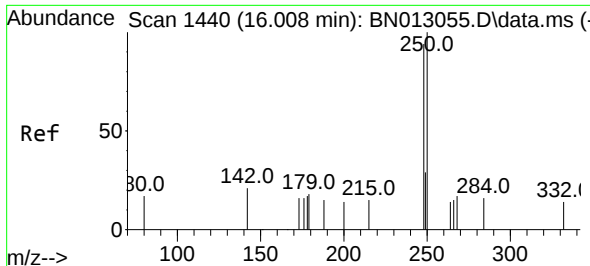

#21
4-Bromophenyl-phenylether
Concen: 0.84 ng
RT: 16.008 min Scan# 1440
Delta R.T. -0.000 min
Lab File: BN013063.D
Acq: 11 Dec 2020 11:45




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4


Tgt Ion:	248	Resp:	507
Ion	Ratio	Lower	Upper
248	100		
250	103.6	77.3	115.9
141	61.4	57.8	86.8

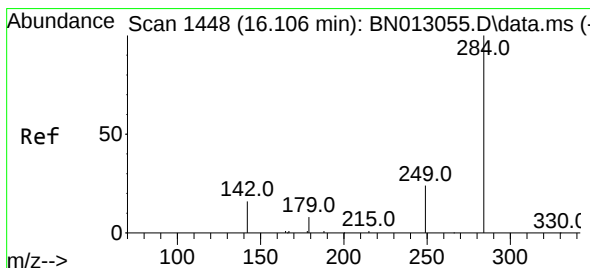

#22
Hexachlorobenzene
Concen: 0.40 ng
RT: 16.105 min Scan# 1448
Delta R.T. -0.000 min
Lab File: BN013063.D
Acq: 11 Dec 2020 11:45

Tgt Ion:	284	Resp:	767
Ion	Ratio	Lower	Upper
284	100		
142	39.5	32.0	48.0
249	32.2	27.0	40.6









#23
Atrazine
Concen: 0.38 ng
RT: 16.288 min Scan# 1463
Delta R.T. -0.000 min
Lab File: BN013063.D
Acq: 11 Dec 2020 11:45




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4


Tgt Ion:200 Resp: 588
Ion Ratio Lower Upper
200 100
173 37.3 22.8 34.2#
215 50.2 38.1 57.1



#24
Pentachlorophenol
Concen: 0.35 ng
RT: 16.471 min Scan# 1478
Delta R.T. 0.012 min
Lab File: BN013063.D
Acq: 11 Dec 2020 11:45

Tgt Ion:266 Resp: 282
Ion Ratio Lower Upper
266 100
264 59.9 50.9 76.3
268 64.2 51.5 77.3









#25
Phenanthrene
Concen: 0.38 ng
RT: 16.836 min Scan# 1508
Delta R.T. -0.000 min
Lab File: BN013063.D
Acq: 11 Dec 2020 11:45




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4


Tgt Ion:178 Resp: 3272
Ion Ratio Lower Upper
178 100
176 19.5 14.8 22.2
179 15.2 12.4 18.6



#26
Anthracene
Concen: 0.37 ng
RT: 16.933 min Scan# 1516
Delta R.T. -0.000 min
Lab File: BN013063.D
Acq: 11 Dec 2020 11:45

Tgt Ion:178 Resp: 2819
Ion Ratio Lower Upper
178 100
176 17.9 14.8 22.2
179 15.2 12.5 18.7









#27
Fluoranthene-d10
Concen: 0.38 ng
RT: 18.843 min Scan# 1773
Delta R.T. -0.000 min
Lab File: BN013063.D
Acq: 11 Dec 2020 11:45




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4


Tgt Ion:212 Resp: 3320
Ion Ratio Lower Upper
212 100
106 9.1 6.8 10.2
104 5.2 4.1 6.1



#28
Fluoranthene
Concen: 0.38 ng
RT: 18.873 min Scan# 1779
Delta R.T. -0.000 min
Lab File: BN013063.D
Acq: 11 Dec 2020 11:45

Tgt Ion:202 Resp: 3967
Ion Ratio Lower Upper
202 100
101 7.2 5.8 8.6
203 17.4 13.7 20.5





#29

Chrysene-d12

Concen: 0.40 ng

RT: 21.024 min Scan# 2103

Delta R.T. 0.010 min

Lab File: BN013063.D

Acq: 11 Dec 2020 11:45

Tgt Ion:240 Resp: 2746

Ion Ratio Lower Upper

240 100

120 10.2 5.3 7.9#





236 28.1 21.8 32.8

Instrument :

BNA_N

ClientSampleId :

SSTDCCC0.4



#30

Pyrene

Concen: 0.39 ng

RT: 19.240 min Scan# 1853

Delta R.T. -0.000 min

Lab File: BN013063.D

Acq: 11 Dec 2020 11:45




Tgt Ion:202 Resp: 4068


Ion Ratio Lower Upper

202 100

200 20.4 16.6 24.8

203 17.9 13.8 20.8









#31
Terphenyl-d14
Concen: 0.40 ng
RT: 19.463 min Scan# 1898
Delta R.T. 0.005 min
Lab File: BN013063.D
Acq: 11 Dec 2020 11:45




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4


Tgt Ion:244 Resp: 2715
Ion Ratio Lower Upper
244 100
212 11.2 7.3 10.9#
122 11.9 7.3 10.9#



#32
Benzo(a)anthracene
Concen: 0.37 ng
RT: 21.003 min Scan# 2101
Delta R.T. -0.000 min
Lab File: BN013063.D
Acq: 11 Dec 2020 11:45

Tgt Ion:228 Resp: 3748
Ion Ratio Lower Upper
228 100
226 28.0 22.3 33.5
229 21.4 15.7 23.5



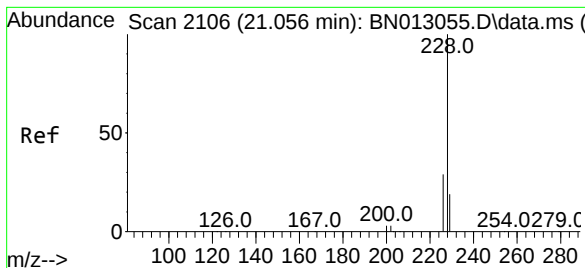

#33

Chrysene

Concen: 0.40 ng

RT: 21.056 min Scan# 2106

Delta R.T. -0.000 min

Lab File: BN013063.D

Acq: 11 Dec 2020 11:45





Instrument :

BNA_N

ClientSampleId :

SSTDCCC0.4

Tgt Ion:	228	Resp:	4174
Ion Ratio	Lower	Upper	
228	100		
226	30.4	24.2	36.2
229	20.4	15.7	23.5



#34

Bis(2-ethylhexyl)phthalate

Concen: 0.30 ng




RT: 20.950 min Scan# 2096


Delta R.T. -0.000 min

Lab File: BN013063.D

Acq: 11 Dec 2020 11:45

Tgt Ion:	149	Resp:	1851
Ion Ratio	Lower	Upper	
149	100		
167	27.0	23.2	34.8
279	4.8	3.9	5.9









#35
Indeno(1,2,3-cd)pyrene
Concen: 0.39 ng
RT: 25.167 min Scan# 3040
Delta R.T. -0.004 min
Lab File: BN013063.D
Acq: 11 Dec 2020 11:45




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4


Tgt Ion:276 Resp: 5433
Ion Ratio Lower Upper
276 100
138 15.6 13.3 19.9
277 23.2 20.2 30.4



#36
Perylene-d12
Concen: 0.40 ng
RT: 23.117 min Scan# 2441
Delta R.T. -0.000 min
Lab File: BN013063.D
Acq: 11 Dec 2020 11:45

Tgt Ion:264 Resp: 2981
Ion Ratio Lower Upper
264 100
260 28.4 19.8 29.6
265 92.3 51.4 77.0#









#37
Benzo(b)fluoranthene
Concen: 0.39 ng
RT: 22.501 min Scan# 2261
Delta R.T. -0.000 min
Lab File: BN013063.D
Acq: 11 Dec 2020 11:45




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4


Tgt Ion:252 Resp: 4366
Ion Ratio Lower Upper
252 100
253 30.1 20.1 30.1
125 11.9 7.2 10.8#



#38
Benzo(k)fluoranthene
Concen: 0.40 ng
RT: 22.542 min Scan# 2273
Delta R.T. -0.000 min
Lab File: BN013063.D
Acq: 11 Dec 2020 11:45

Tgt Ion:252 Resp: 4737
Ion Ratio Lower Upper
252 100
253 30.7 19.8 29.8#
125 12.4 7.1 10.7#









#39
Benzo(a)pyrene
Concen: 0.39 ng
RT: 23.028 min Scan# 2415
Delta R.T. -0.000 min
Lab File: BN013063.D
Acq: 11 Dec 2020 11:45




Instrument :
BNA_N
ClientSampleId :
SSTDCCC0.4


Tgt Ion:252 Resp: 4228
Ion Ratio Lower Upper
252 100
253 33.9 21.3 31.9#
125 16.0 8.3 12.5#



#40
Dibenzo(a,h)anthracene
Concen: 0.39 ng
RT: 25.188 min Scan# 3046
Delta R.T. 0.003 min
Lab File: BN013063.D
Acq: 11 Dec 2020 11:45

Tgt Ion:278 Resp: 4645
Ion Ratio Lower Upper
278 100
139 14.8 9.3 13.9#
279 32.9 21.6 32.4#



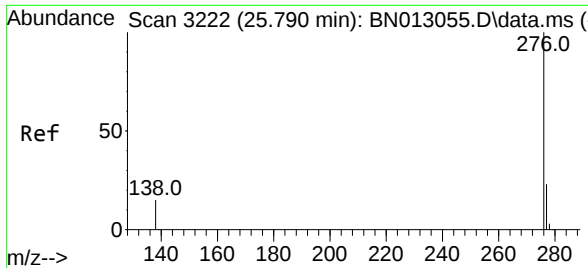

#41
 Benzo(g,h,i)perylene
 Concen: 0.41 ng
 RT: 25.790 min Scan# 3222
 Delta R.T. -0.000 min
 Lab File: BN013063.D
 Acq: 11 Dec 2020 11:45

Instrument :
 BNA_N
 ClientSampleId :
 SSTDCCC0.4

Tgt Ion:	276	Resp:	5085
Ion Ratio	Lower	Upper	
276	100		
277	26.8	19.8	29.8
138	18.5	11.7	17.5#

