
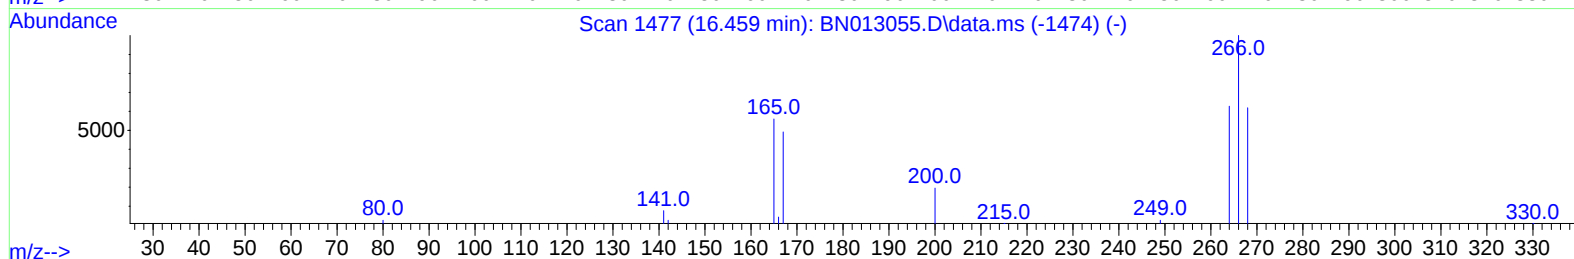
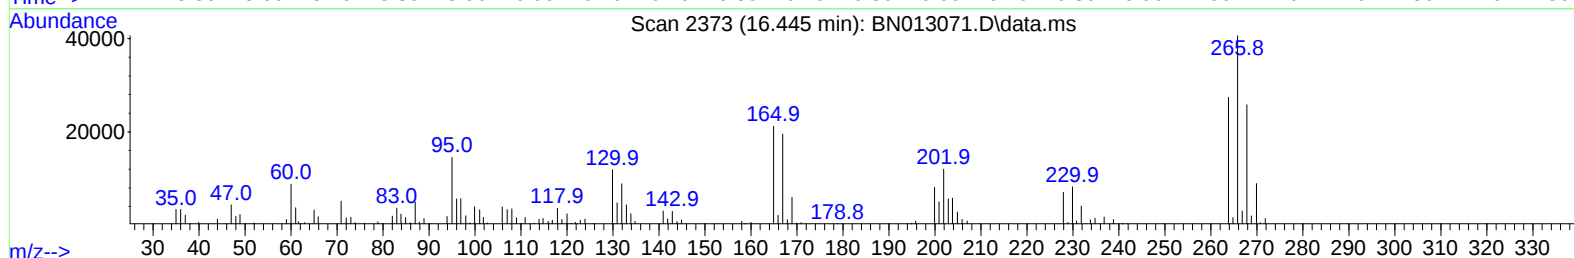


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121120\
Data File : BN013071.D
Acq On : 12 Dec 2020 02:20
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 12 02:51:59 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN121020.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 11 01:53:51 2020
Response via : Initial Calibration

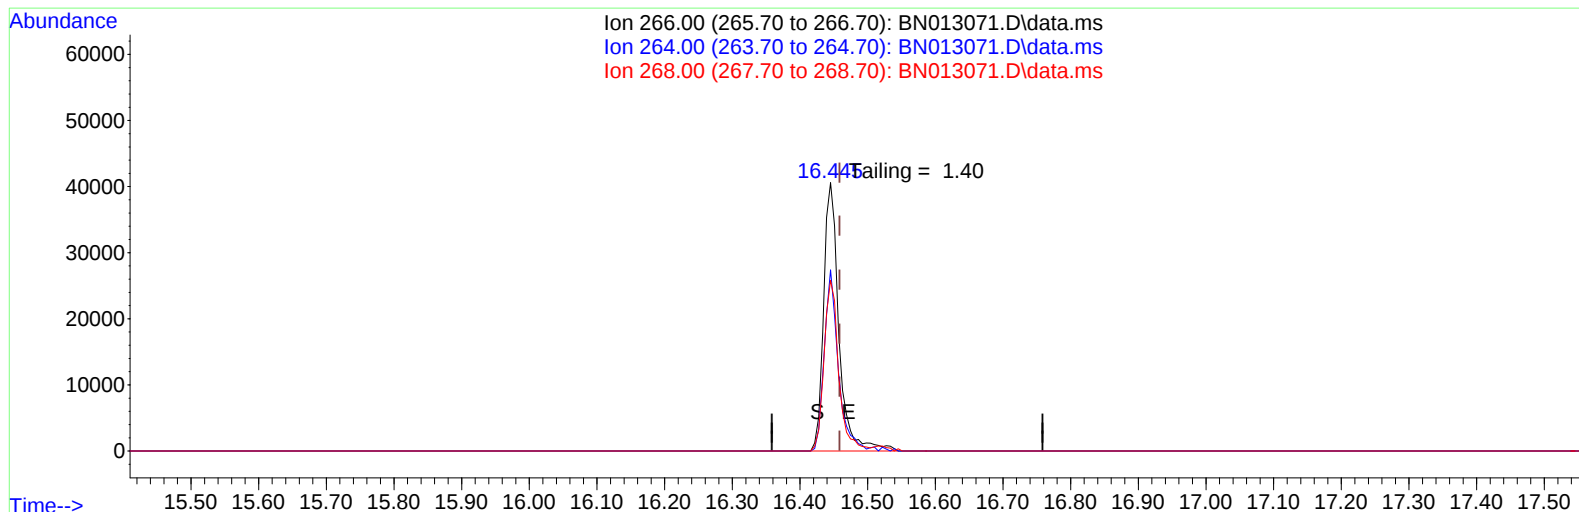

TIC: BN013071.D\data.ms

(24) Pentachlorophenol

16.445min (-0.013) 0.00 ng

response 63951

Ion	Exp%	Act%
266.00	100.00	100.00
264.00	63.60	62.45
268.00	64.40	61.00
0.00	0.00	0.00