

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121120\
 Data File : BN013069.D
 Acq On : 11 Dec 2020 15:22
 Operator : CG/JU
 Sample : L4960-02
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 MW-6

Quant Time: Dec 11 17:28:40 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN121020.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Dec 11 01:53:51 2020
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.370	152	884	0.40	ng	0.00
7) Naphthalene-d8	10.137	136	3144	0.40	ng	# 0.00
13) Acenaphthene-d10	14.029	164	1896	0.40	ng	0.00
19) Phenanthrene-d10	16.799	188	3910	0.40	ng	# 0.00
29) Chrysene-d12	21.024	240	4322	0.40	ng	# 0.01
36) Perylene-d12	23.113	264	4695	0.40	ng	0.00
System Monitoring Compounds						
4) 2-Fluorophenol	4.994	112	339	0.11	ng	0.00
5) Phenol-d6	6.565	99	230	0.06	ng	0.00
8) Nitrobenzene-d5	8.540	82	975	0.29	ng	0.01
11) 2-Methylnaphthalene-d10	11.742	152	1657	0.29	ng	0.00
14) 2,4,6-Tribromophenol	15.551	330	313	0.25	ng	0.00
15) 2-Fluorobiphenyl	12.646	172	2639	0.32	ng	0.00
27) Fluoranthene-d10	18.843	212	4953	0.38	ng	0.00
31) Terphenyl-d14	19.459	244	4683	0.43	ng	0.00
Target Compounds						
34) Bis(2-ethylhexyl)phtha...	20.950	149	1021	0.11	ng	Qvalue 94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121120\
Data File : BN013069.D
Acq On : 11 Dec 2020 15:22
Operator : CG/JU
Sample : L4960-02
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
MW-6

Quant Time: Dec 11 17:28:40 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN121020.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 11 01:53:51 2020
Response via : Initial Calibration




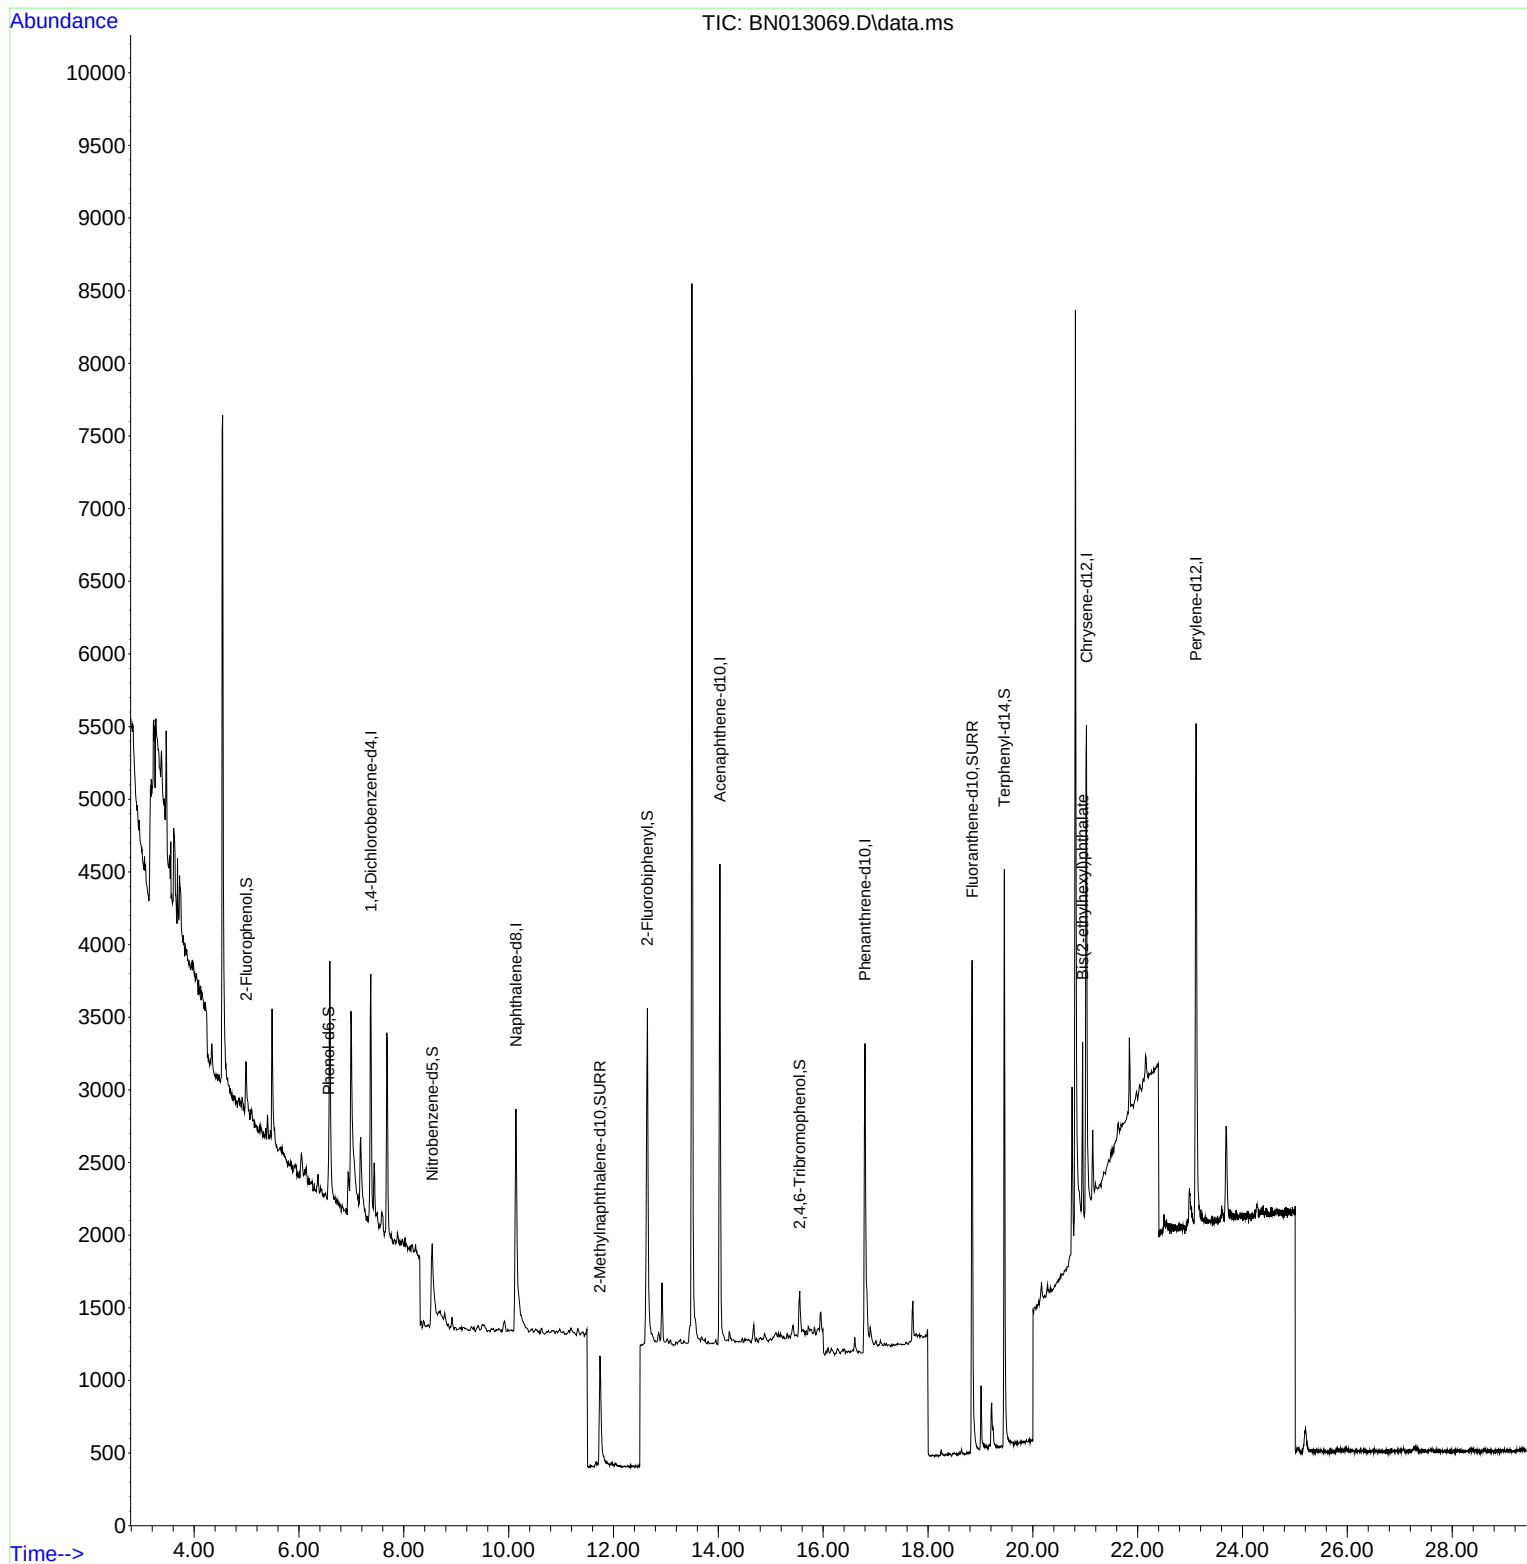


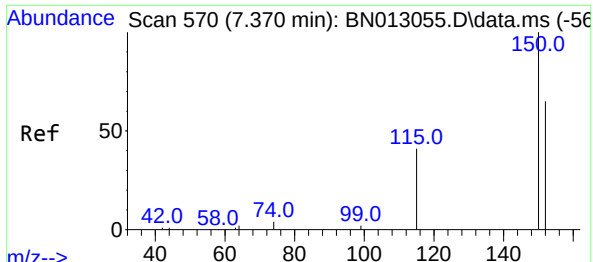

#1
1,4-Dichlorobenzene-d4
Concen: 0.40 ng
RT: 7.370 min Scan# 570
Delta R.T. 0.000 min
Lab File: BN013069.D
Acq: 11 Dec 2020 15:22




Instrument :
BNA_N
ClientSampled :
MW-6


Tgt Ion:152 Resp: 884
Ion Ratio Lower Upper
152 100
150 151.9 116.6 174.8
115 73.1 52.9 79.3

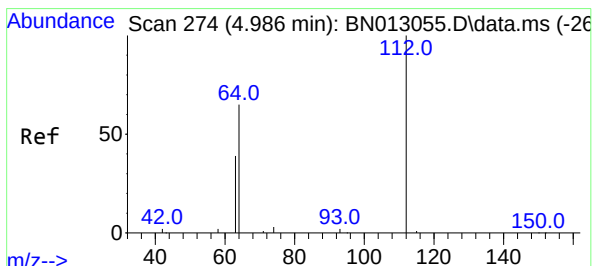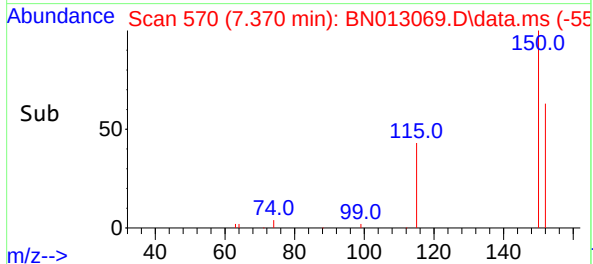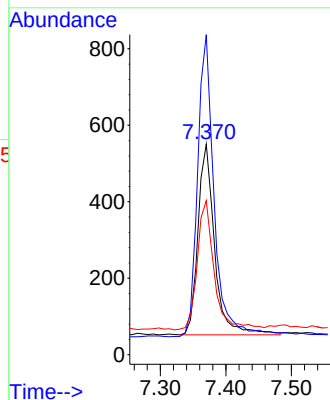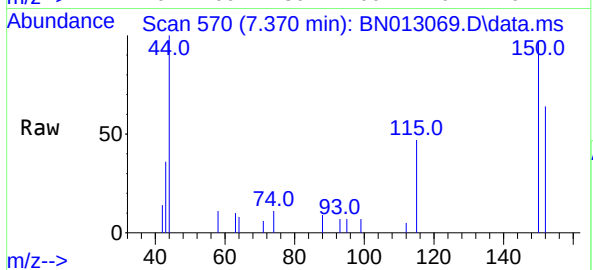

#4
2-Fluorophenol
Concen: 0.11 ng
RT: 4.994 min Scan# 275
Delta R.T. 0.008 min
Lab File: BN013069.D
Acq: 11 Dec 2020 15:22

Tgt Ion:112 Resp: 339
Ion Ratio Lower Upper
112 100
64 66.7 49.5 74.3
63 37.8 32.0 48.0


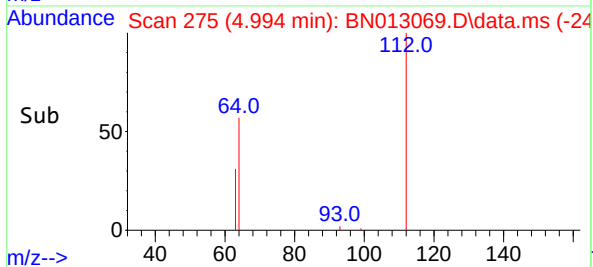
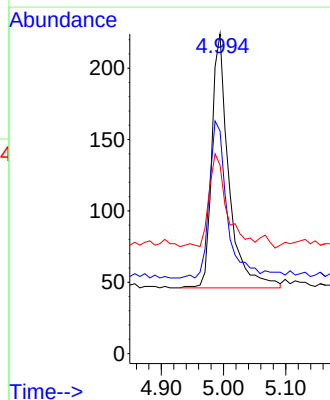
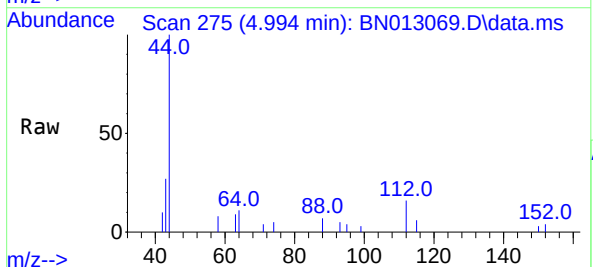


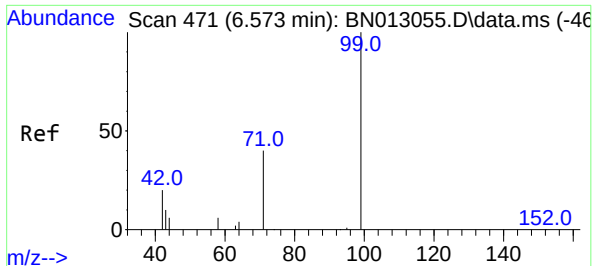

#5
Phenol-d6
Concen: 0.06 ng
RT: 6.565 min Scan# 470
Delta R.T. -0.008 min
Lab File: BN013069.D
Acq: 11 Dec 2020 15:22




Instrument :
BNA_N
ClientSampleId :
MW-6


Tgt Ion: 99 Resp: 230
Ion Ratio Lower Upper
99 100
42 101.7 22.4 33.6#
71 46.5 37.8 56.6

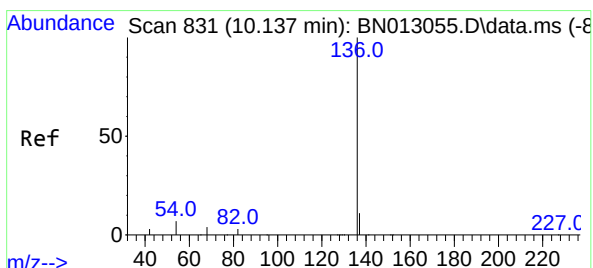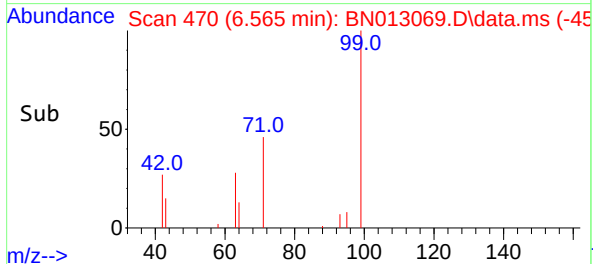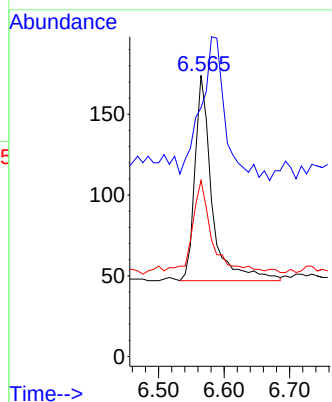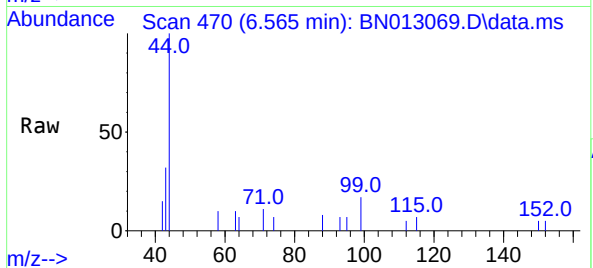

#7
Naphthalene-d8
Concen: 0.40 ng
RT: 10.137 min Scan# 831
Delta R.T. -0.000 min
Lab File: BN013069.D
Acq: 11 Dec 2020 15:22

Tgt Ion: 136 Resp: 3144
Ion Ratio Lower Upper
136 100
137 14.3 10.6 15.8
54 12.5 8.6 12.8
68 9.2 5.7 8.5#


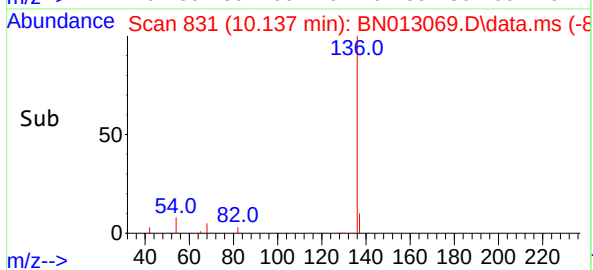
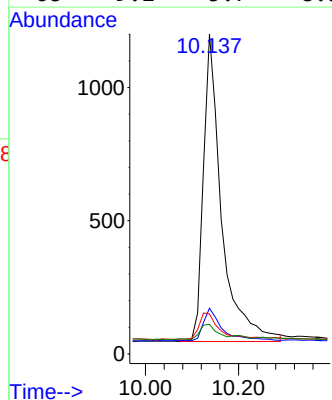
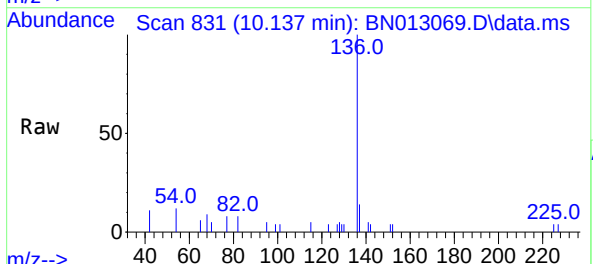




#8
Nitrobenzene-d5
Concen: 0.29 ng
RT: 8.540 min Scan# 705
Delta R.T. 0.012 min
Lab File: BN013069.D
Acq: 11 Dec 2020 15:22




Instrument :
BNA_N
ClientSampleId :
MW-6


Tgt Ion: 82 Resp: 975
Ion Ratio Lower Upper
82 100
128 50.0 30.6 46.0#
54 66.2 48.3 72.5

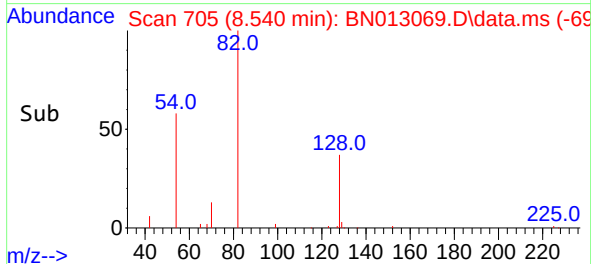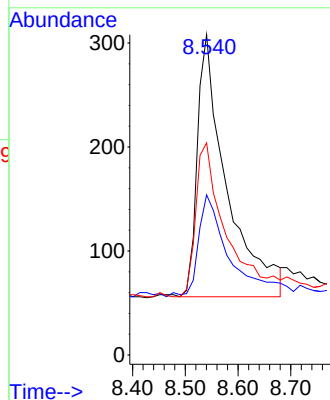

#11
2-Methylnaphthalene-d10
Concen: 0.29 ng
RT: 11.742 min Scan# 992
Delta R.T. -0.000 min
Lab File: BN013069.D
Acq: 11 Dec 2020 15:22

Tgt Ion: 152 Resp: 1657
Ion Ratio Lower Upper
152 100
151 21.1 16.7 25.1


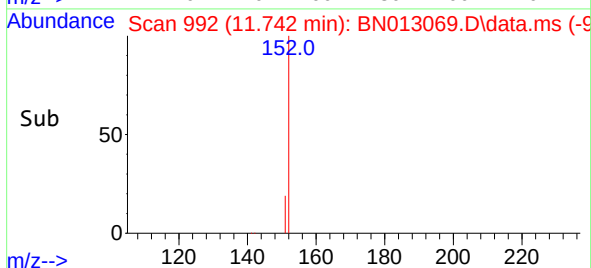
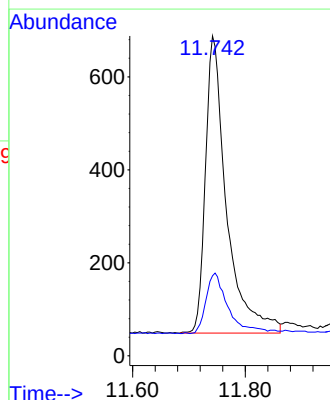
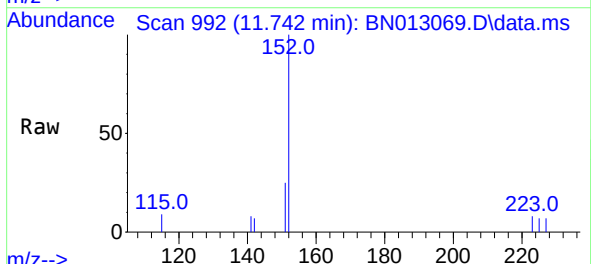




#13
Acenaphthene-d10
Concen: 0.40 ng
RT: 14.029 min Scan# 1284
Delta R.T. -0.000 min
Lab File: BN013069.D
Acq: 11 Dec 2020 15:22




Instrument :
BNA_N
ClientSampleId :
MW-6


Tgt Ion:	164	Resp:	1896
Ion	Ratio	Lower	Upper
164	100		
162	106.0	80.6	120.8
160	51.3	39.5	59.3

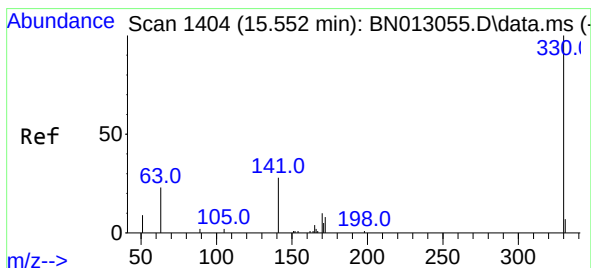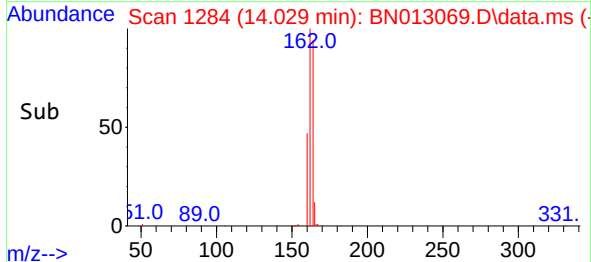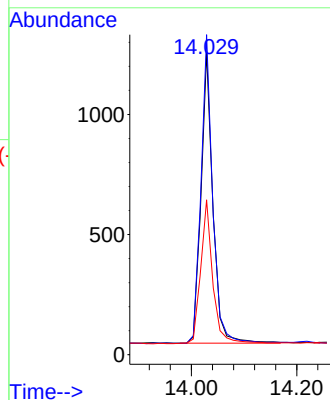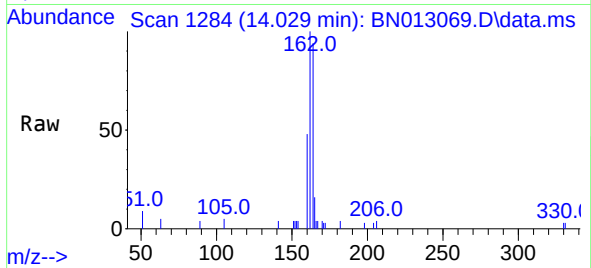

#14
2,4,6-Tribromophenol
Concen: 0.25 ng
RT: 15.551 min Scan# 1404
Delta R.T. -0.000 min
Lab File: BN013069.D
Acq: 11 Dec 2020 15:22

Tgt Ion:	330	Resp:	313
Ion	Ratio	Lower	Upper
330	100		
332	0.0	0.0	0.0
141	50.5	34.4	51.6


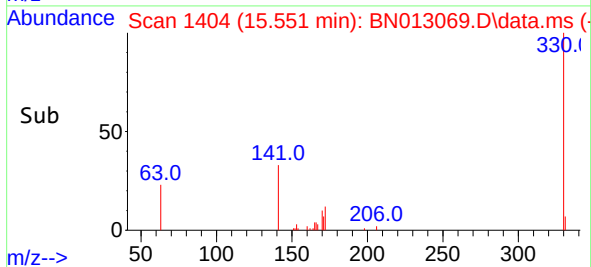
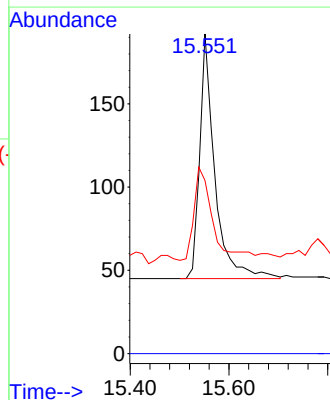
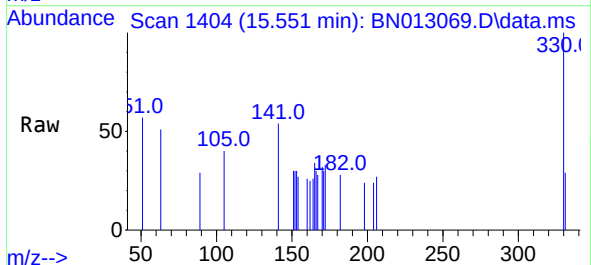




#15
2-Fluorobiphenyl
Concen: 0.32 ng
RT: 12.646 min Scan# 1175
Delta R.T. -0.000 min
Lab File: BN013069.D
Acq: 11 Dec 2020 15:22




Instrument :
BNA_N
ClientSampleId :
MW-6


Tgt Ion:	172	Resp:	2639
Ion	Ratio	Lower	Upper
172	100		
171	37.3	28.2	42.4
170	25.6	20.0	30.0

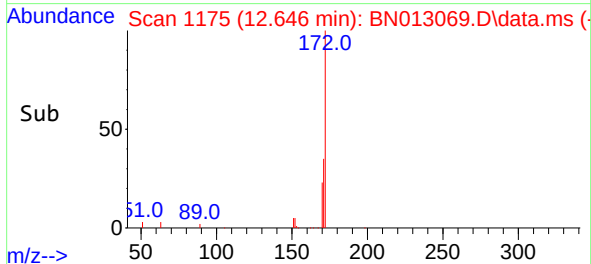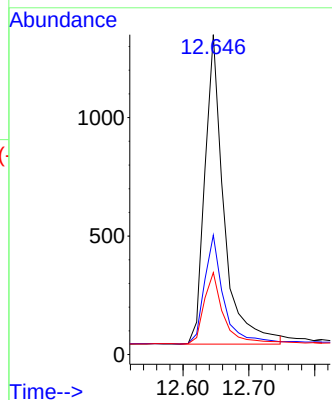

#19
Phenanthrene-d10
Concen: 0.40 ng
RT: 16.799 min Scan# 1505
Delta R.T. -0.000 min
Lab File: BN013069.D
Acq: 11 Dec 2020 15:22

Tgt Ion:	188	Resp:	3910
Ion	Ratio	Lower	Upper
188	100		
94	0.0	0.0	0.0
80	9.3	5.0	7.4#


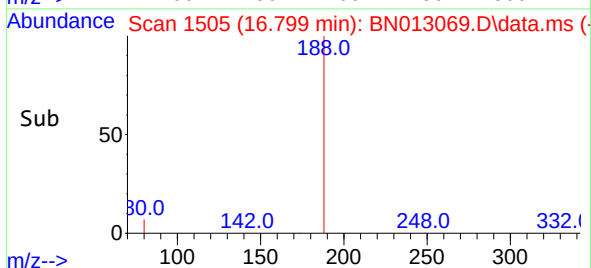
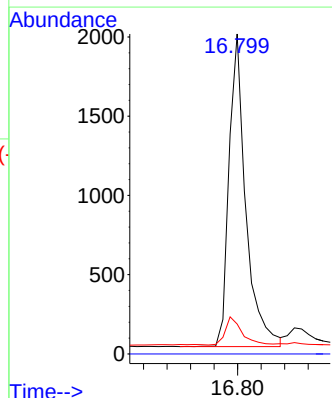
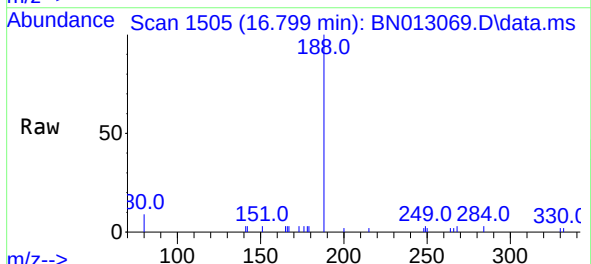




#27
Fluoranthene-d10
Concen: 0.38 ng
RT: 18.843 min Scan# 1773
Delta R.T. -0.000 min
Lab File: BN013069.D
Acq: 11 Dec 2020 15:22




Instrument :
BNA_N
ClientSampleId :
MW-6


Tgt Ion:	212	Resp:	4953
Ion Ratio	Lower	Upper	
212	100		
106	9.5	6.8	10.2
104	5.3	4.1	6.1

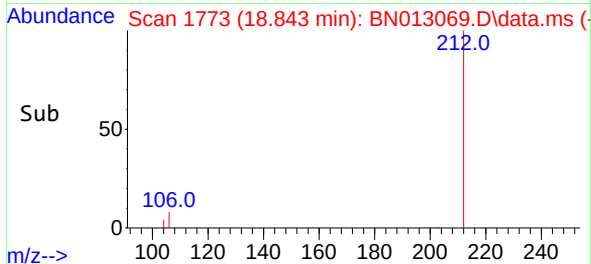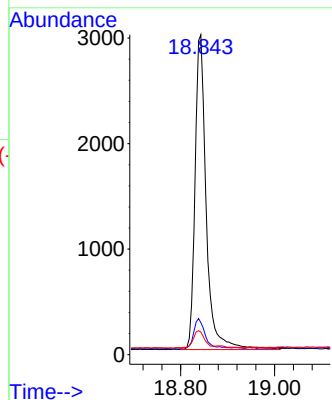

#29
Chrysene-d12
Concen: 0.40 ng
RT: 21.024 min Scan# 2103
Delta R.T. 0.010 min
Lab File: BN013069.D
Acq: 11 Dec 2020 15:22

Tgt Ion:	240	Resp:	4322
Ion Ratio	Lower	Upper	
240	100		
120	9.5	5.3	7.9#
236	28.2	21.8	32.8


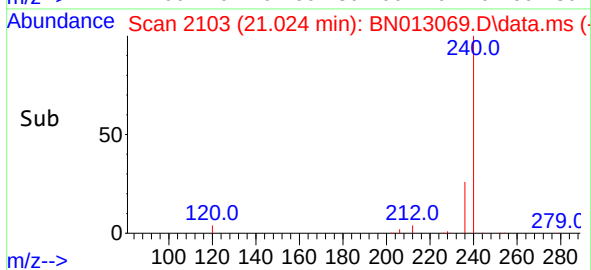
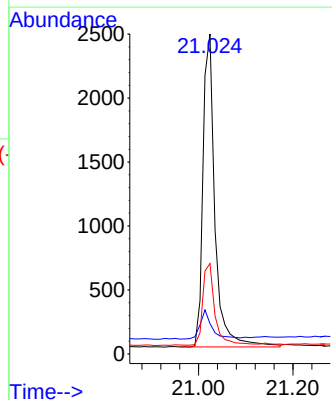
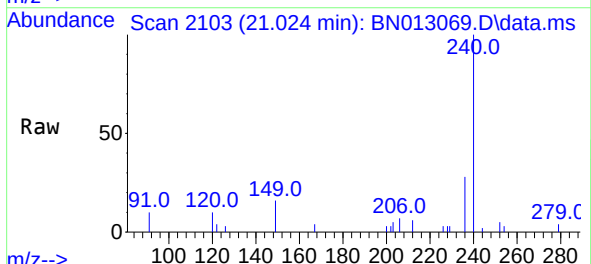




#31
Terphenyl-d14
Concen: 0.43 ng
RT: 19.459 min Scan# 1897
Delta R.T. -0.000 min
Lab File: BN013069.D
Acq: 11 Dec 2020 15:22




Instrument :
BNA_N
ClientSampleId :
MW-6




Tgt Ion:	244	Resp:	4683
Ion	Ratio	Lower	Upper
244	100		
212	9.5	7.3	10.9
122	10.2	7.3	10.9

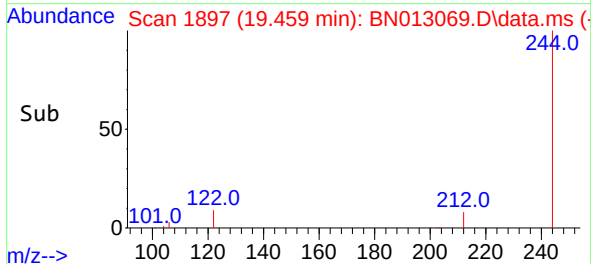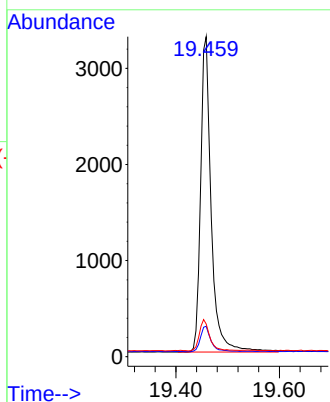

#34
Bis(2-ethylhexyl)phthalate
Concen: 0.11 ng
RT: 20.950 min Scan# 2096
Delta R.T. -0.000 min
Lab File: BN013069.D
Acq: 11 Dec 2020 15:22

Tgt Ion:	149	Resp:	1021
Ion	Ratio	Lower	Upper
149	100		
167	25.2	23.2	34.8
279	5.6	3.9	5.9

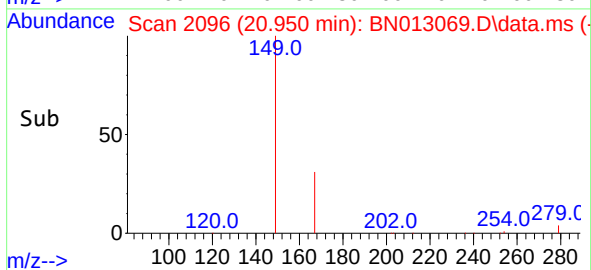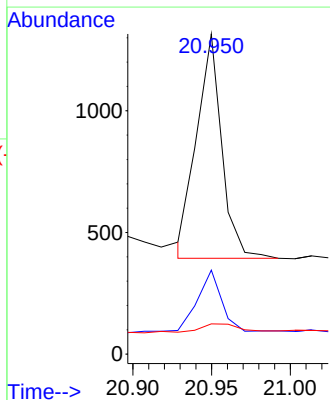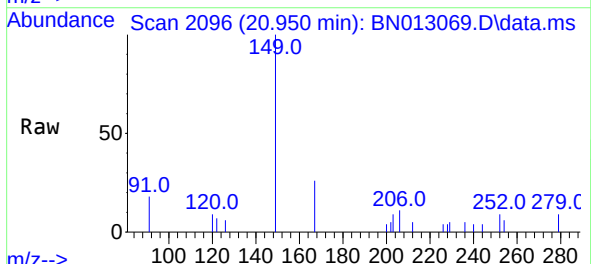


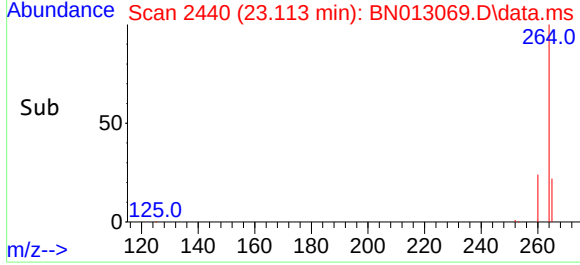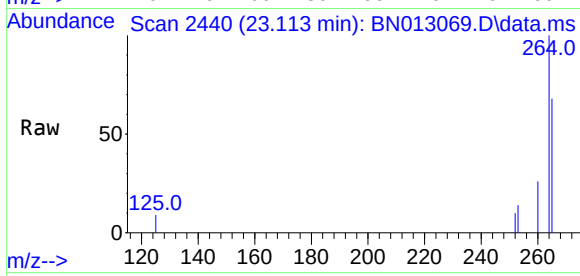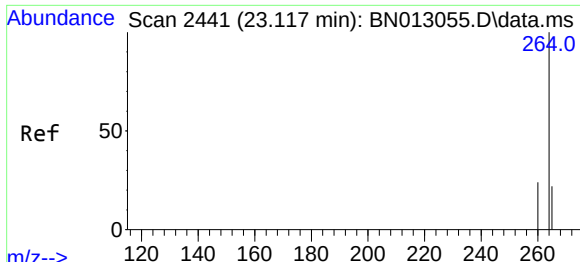

#36
 Perylene-d12
 Concen: 0.40 ng
 RT: 23.113 min Scan# 2440
 Delta R.T. -0.004 min
 Lab File: BN013069.D
 Acq: 11 Dec 2020 15:22

Tgt Ion:264 Resp: 4695

Ion	Ratio	Lower	Upper
264	100		
260	25.7	19.8	29.6
265	67.8	51.4	77.0

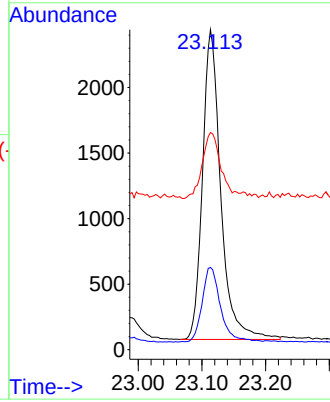

Instrument :
 BNA_N
 ClientSampleId :
 MW-6