


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121120\
Data File : BN013062.D
Acq On : 11 Dec 2020 11:09
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN121020.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Dec 11 01:53:51 2020

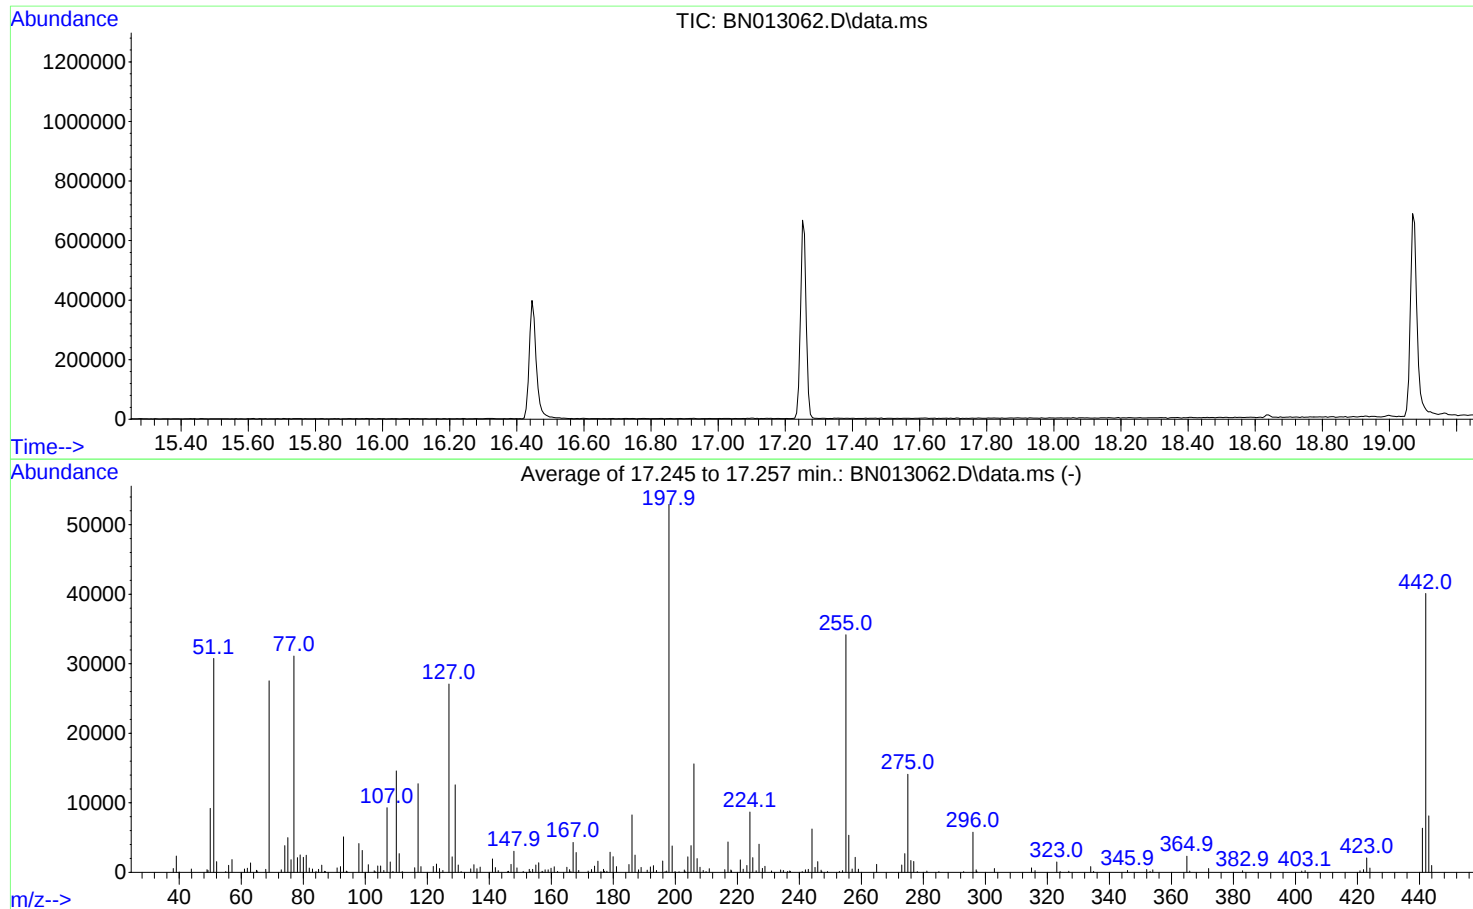

AutoFind: Scans 2509, 2510, 2511; Background Corrected with Scan 2503

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	58.1	30765	PASS
68	69	0.00	2	1.6	439	PASS
69	198	0.00	100	52.1	27549	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	51.2	27077	PASS
197	198	0.00	2	0.3	178	PASS
198	198	100	100	100.0	52909	PASS
199	198	5	9	7.2	3795	PASS
275	198	10	60	26.7	14118	PASS
365	198	1	100	4.4	2325	PASS
441	198	0.01	100	12.0	6353	PASS
442	198	50	100	75.8	40107	PASS
443	442	15	24	20.3	8133	PASS