


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121120\
 Data File : BN013071.D
 Acq On : 12 Dec 2020 02:20
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN121020.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Dec 11 01:53:51 2020

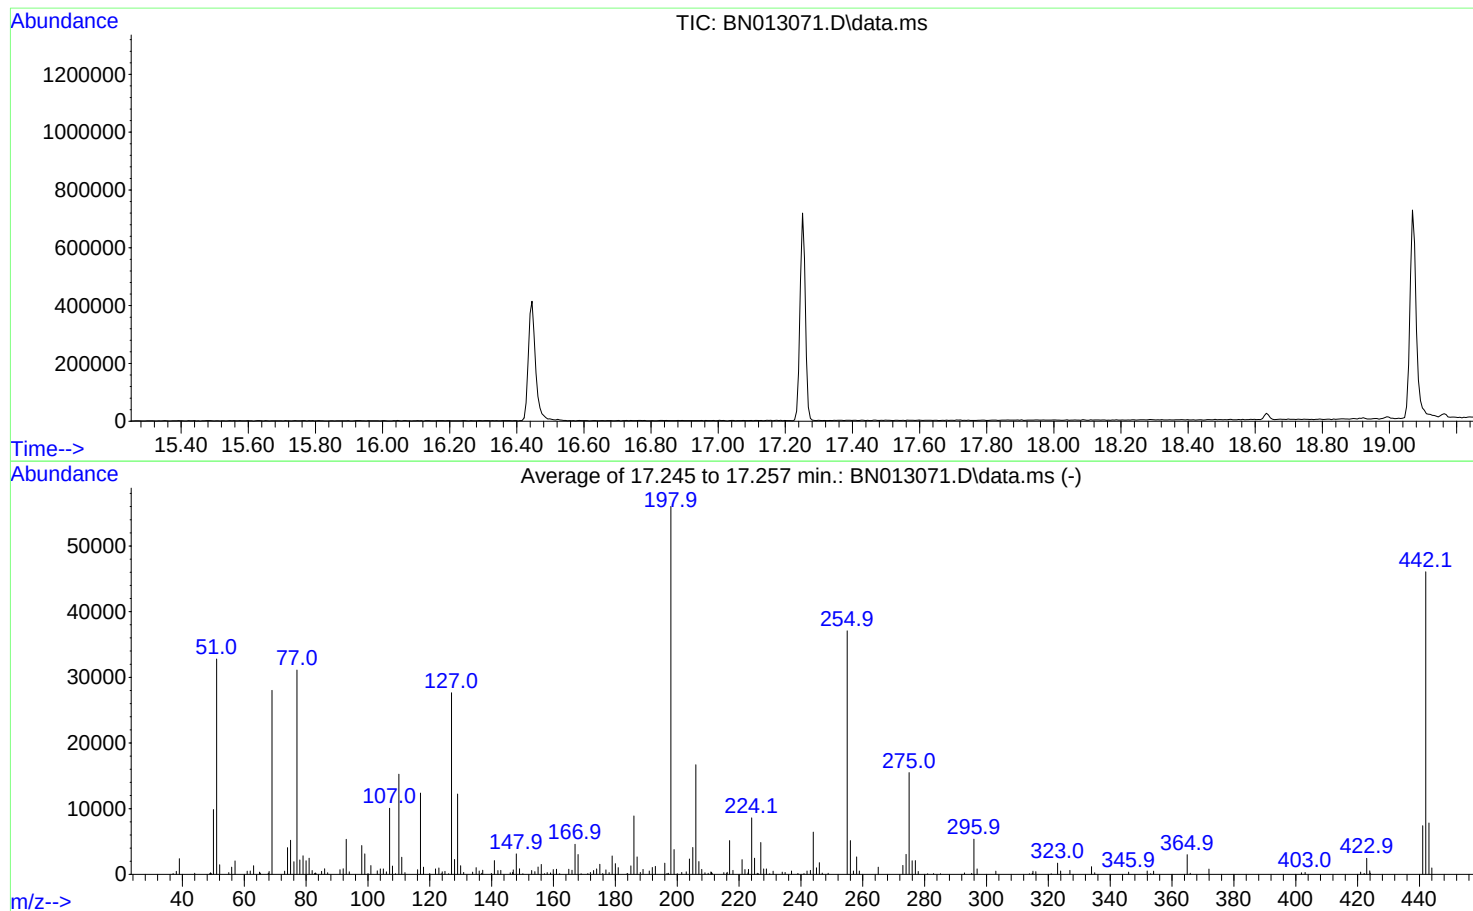

AutoFind: Scans 2509, 2510, 2511; Background Corrected with Scan 2503

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	58.5	32792	PASS
68	69	0.00	2	1.6	441	PASS
69	198	0.00	100	50.0	28029	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	49.4	27664	PASS
197	198	0.00	2	0.3	173	PASS
198	198	100	100	100.0	56011	PASS
199	198	5	9	6.7	3766	PASS
275	198	10	60	27.7	15491	PASS
365	198	1	100	5.4	3005	PASS
441	198	0.01	100	13.2	7415	PASS
442	198	50	100	82.3	46083	PASS
443	442	15	24	17.0	7816	PASS