


2,4,6-Tribromophenol

Response Ratio

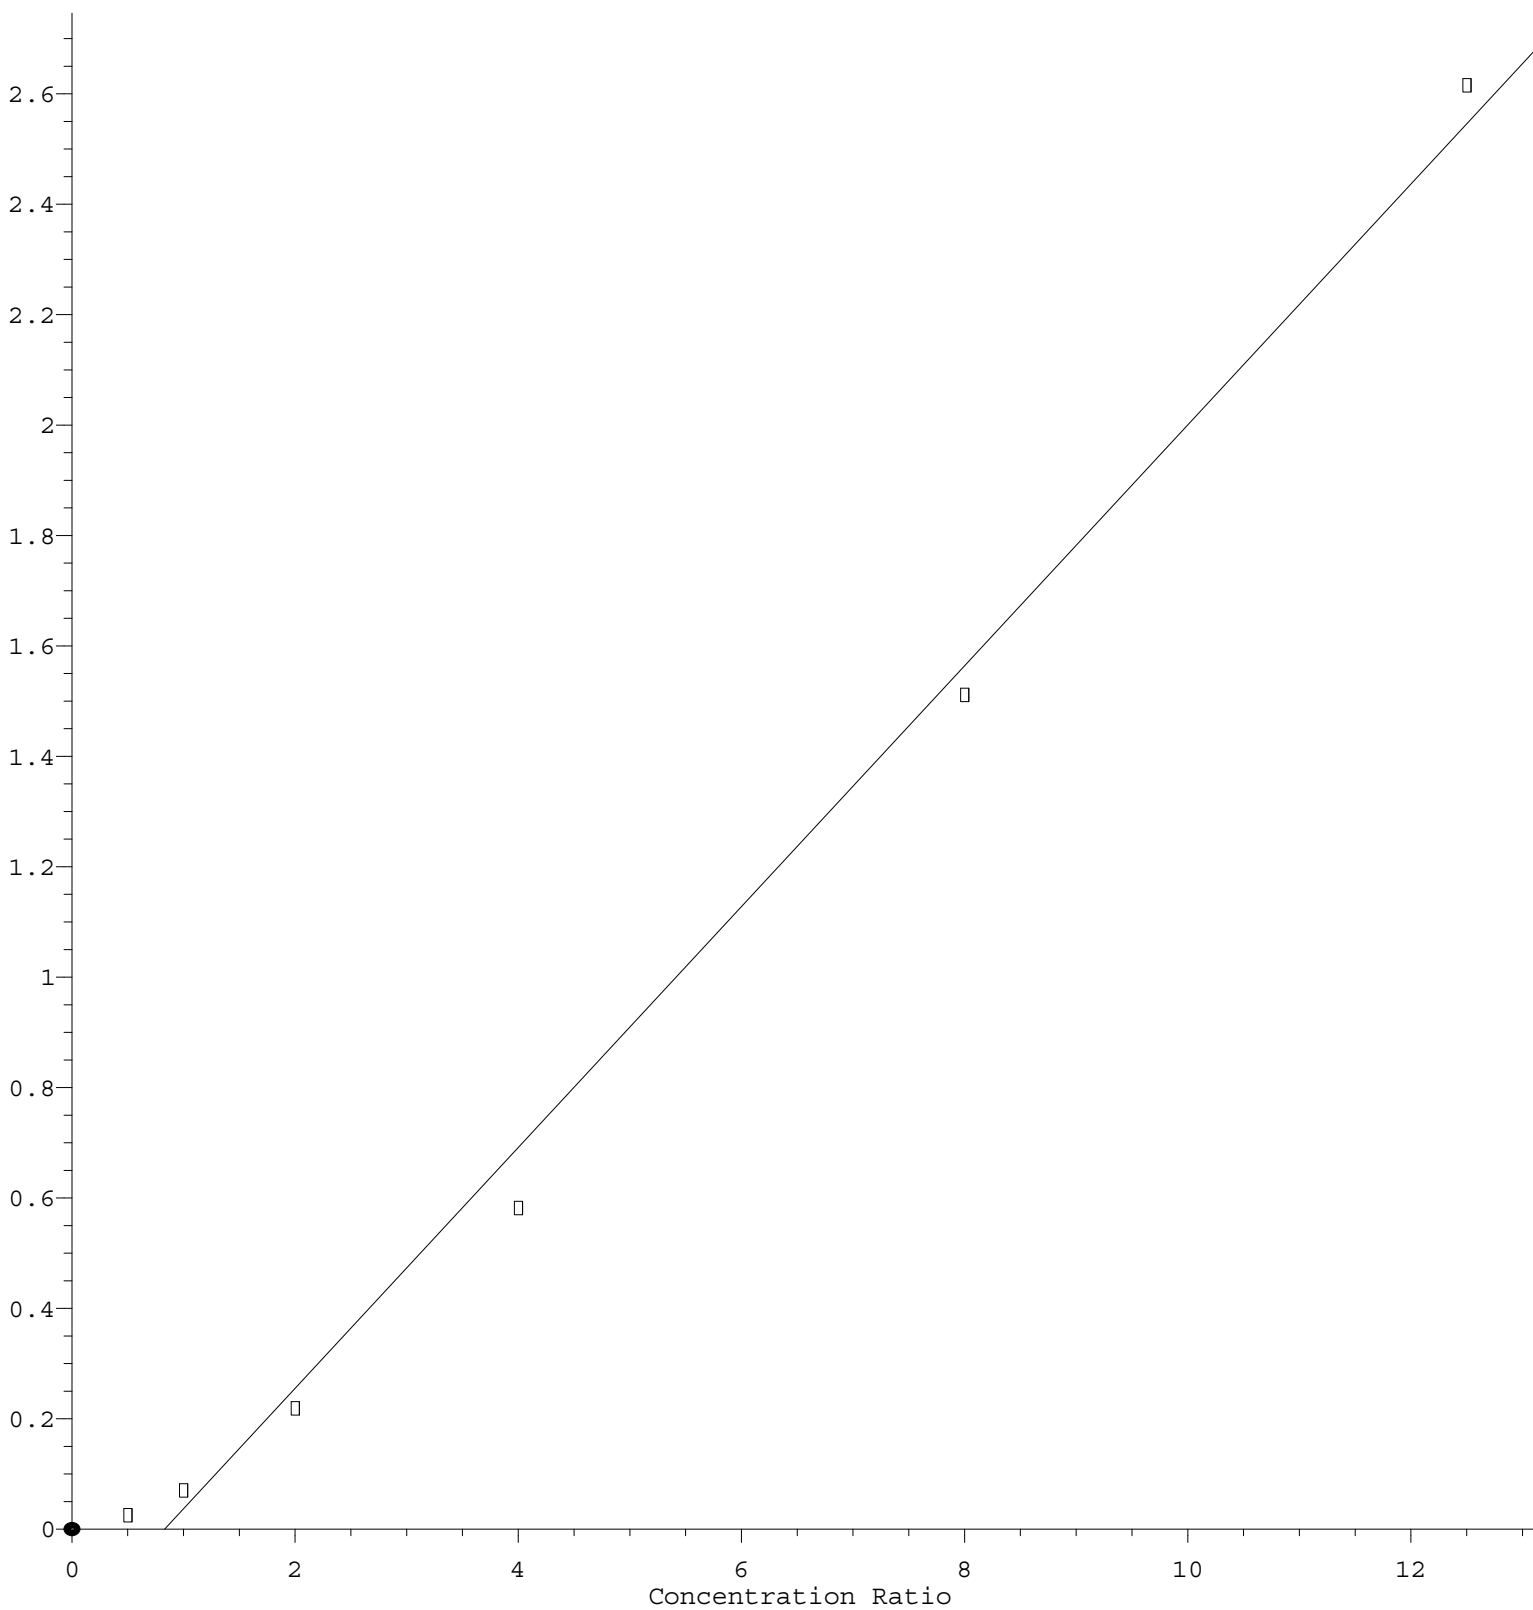


$$\text{Response} = 2.183\text{e-}001 * \text{Amt} - 1.815\text{e-}001$$

Coef of Det (r^2) = 0.994057 Curve Fit: Linear

Method Name: Z:\SVOASRV\HPCHEM1\BNA N\METHODS\8270-SIM-BN121121.M

Calibration Table Last Updated: Sat Dec 11 00:01:30 2021


Atrazine

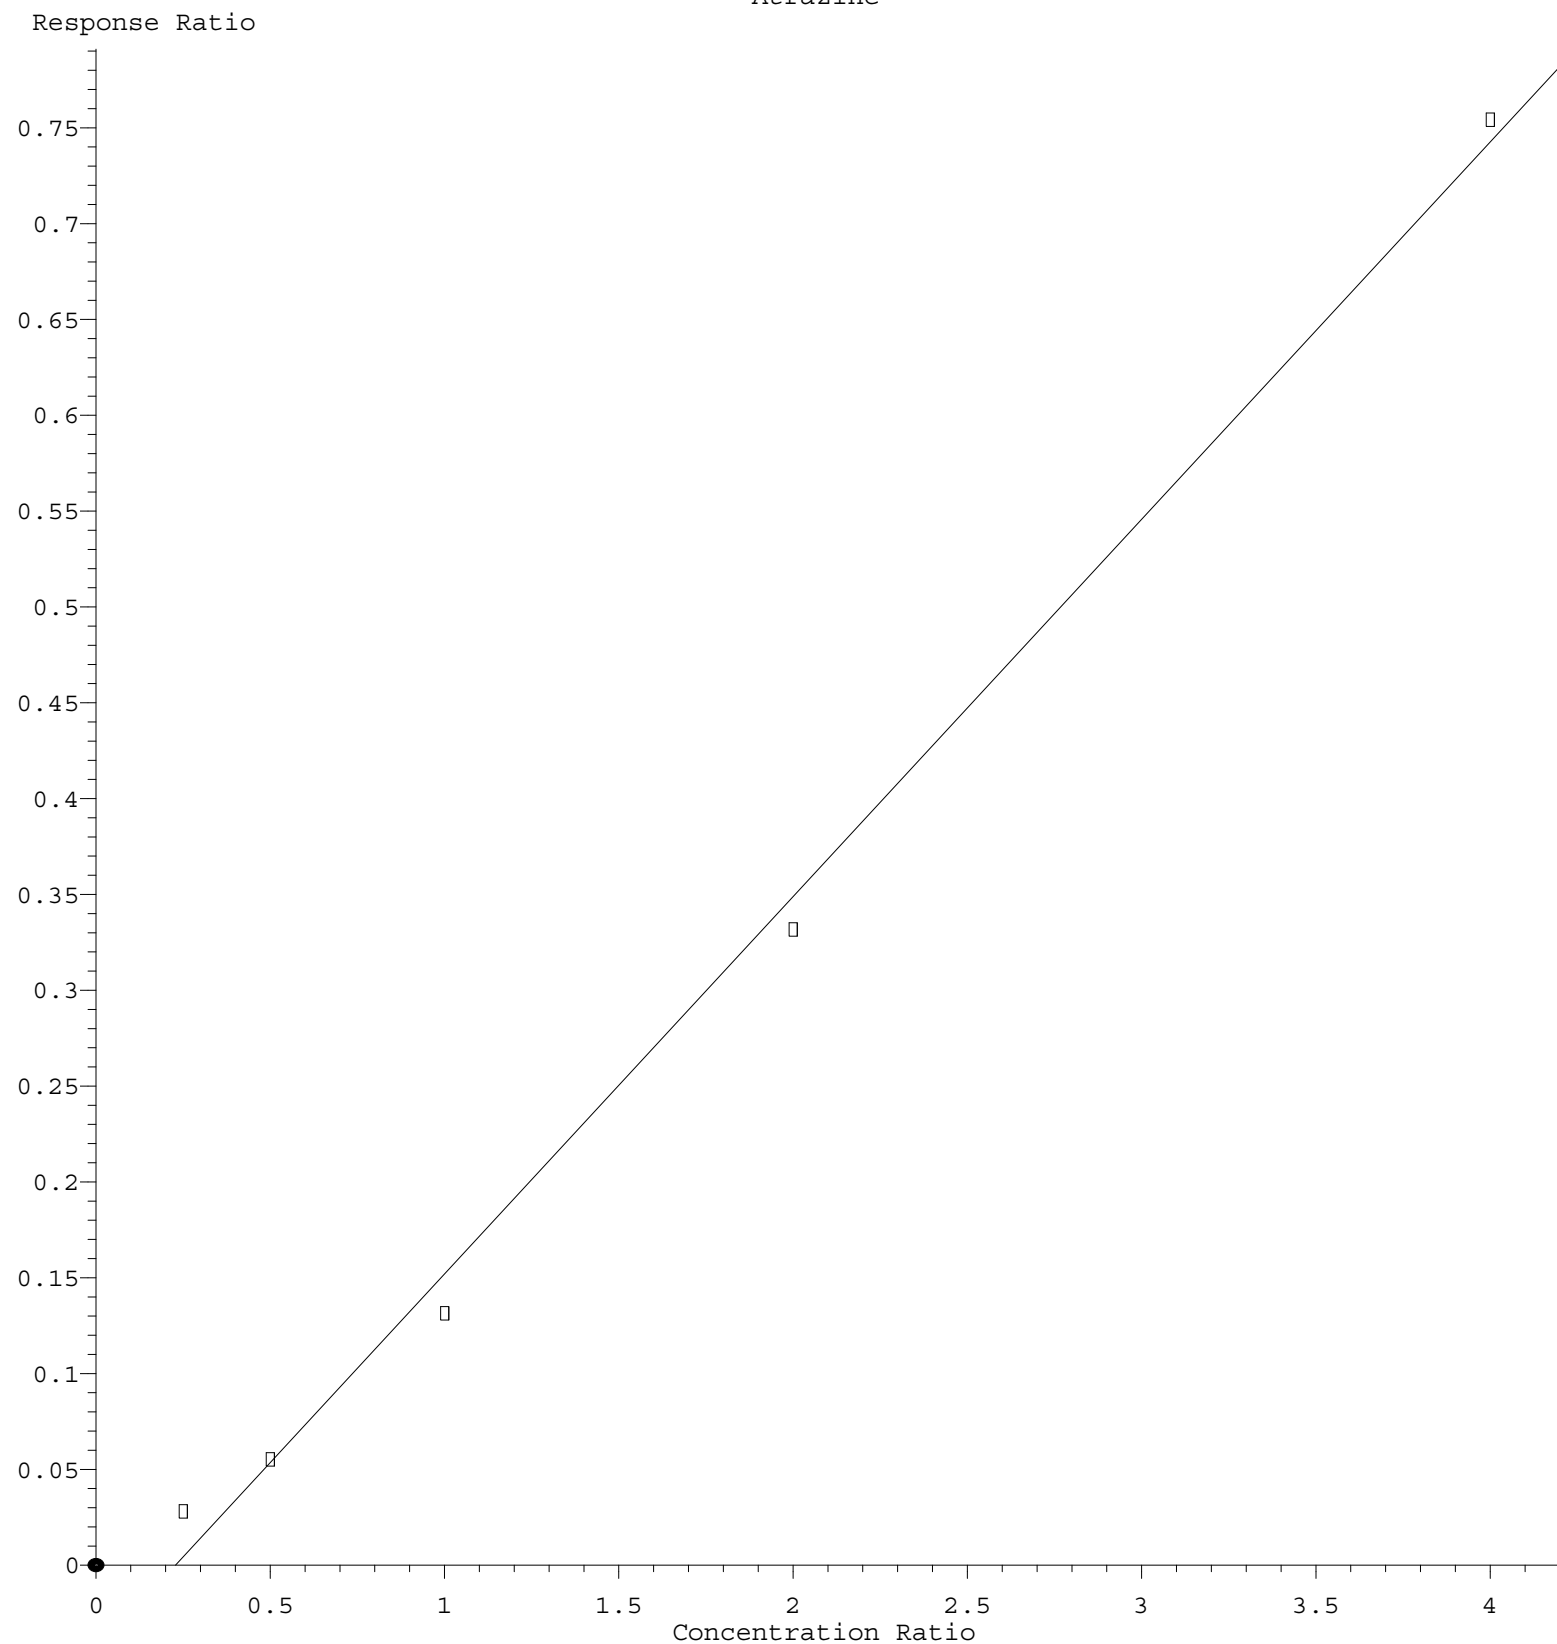

Response = 1.968e-001 * Amt - 4.496e-002
 Coef of Det (r^2) = 0.996075 Curve Fit: Linear
 Method Name: Z:\SVOASRV\HPCHEM1\BNA N\METHODS\8270-SIM-BN121121.M
 Calibration Table Last Updated: Sat Dec 11 00:01:30 2021

Benzo (a) anthracene

Response Ratio

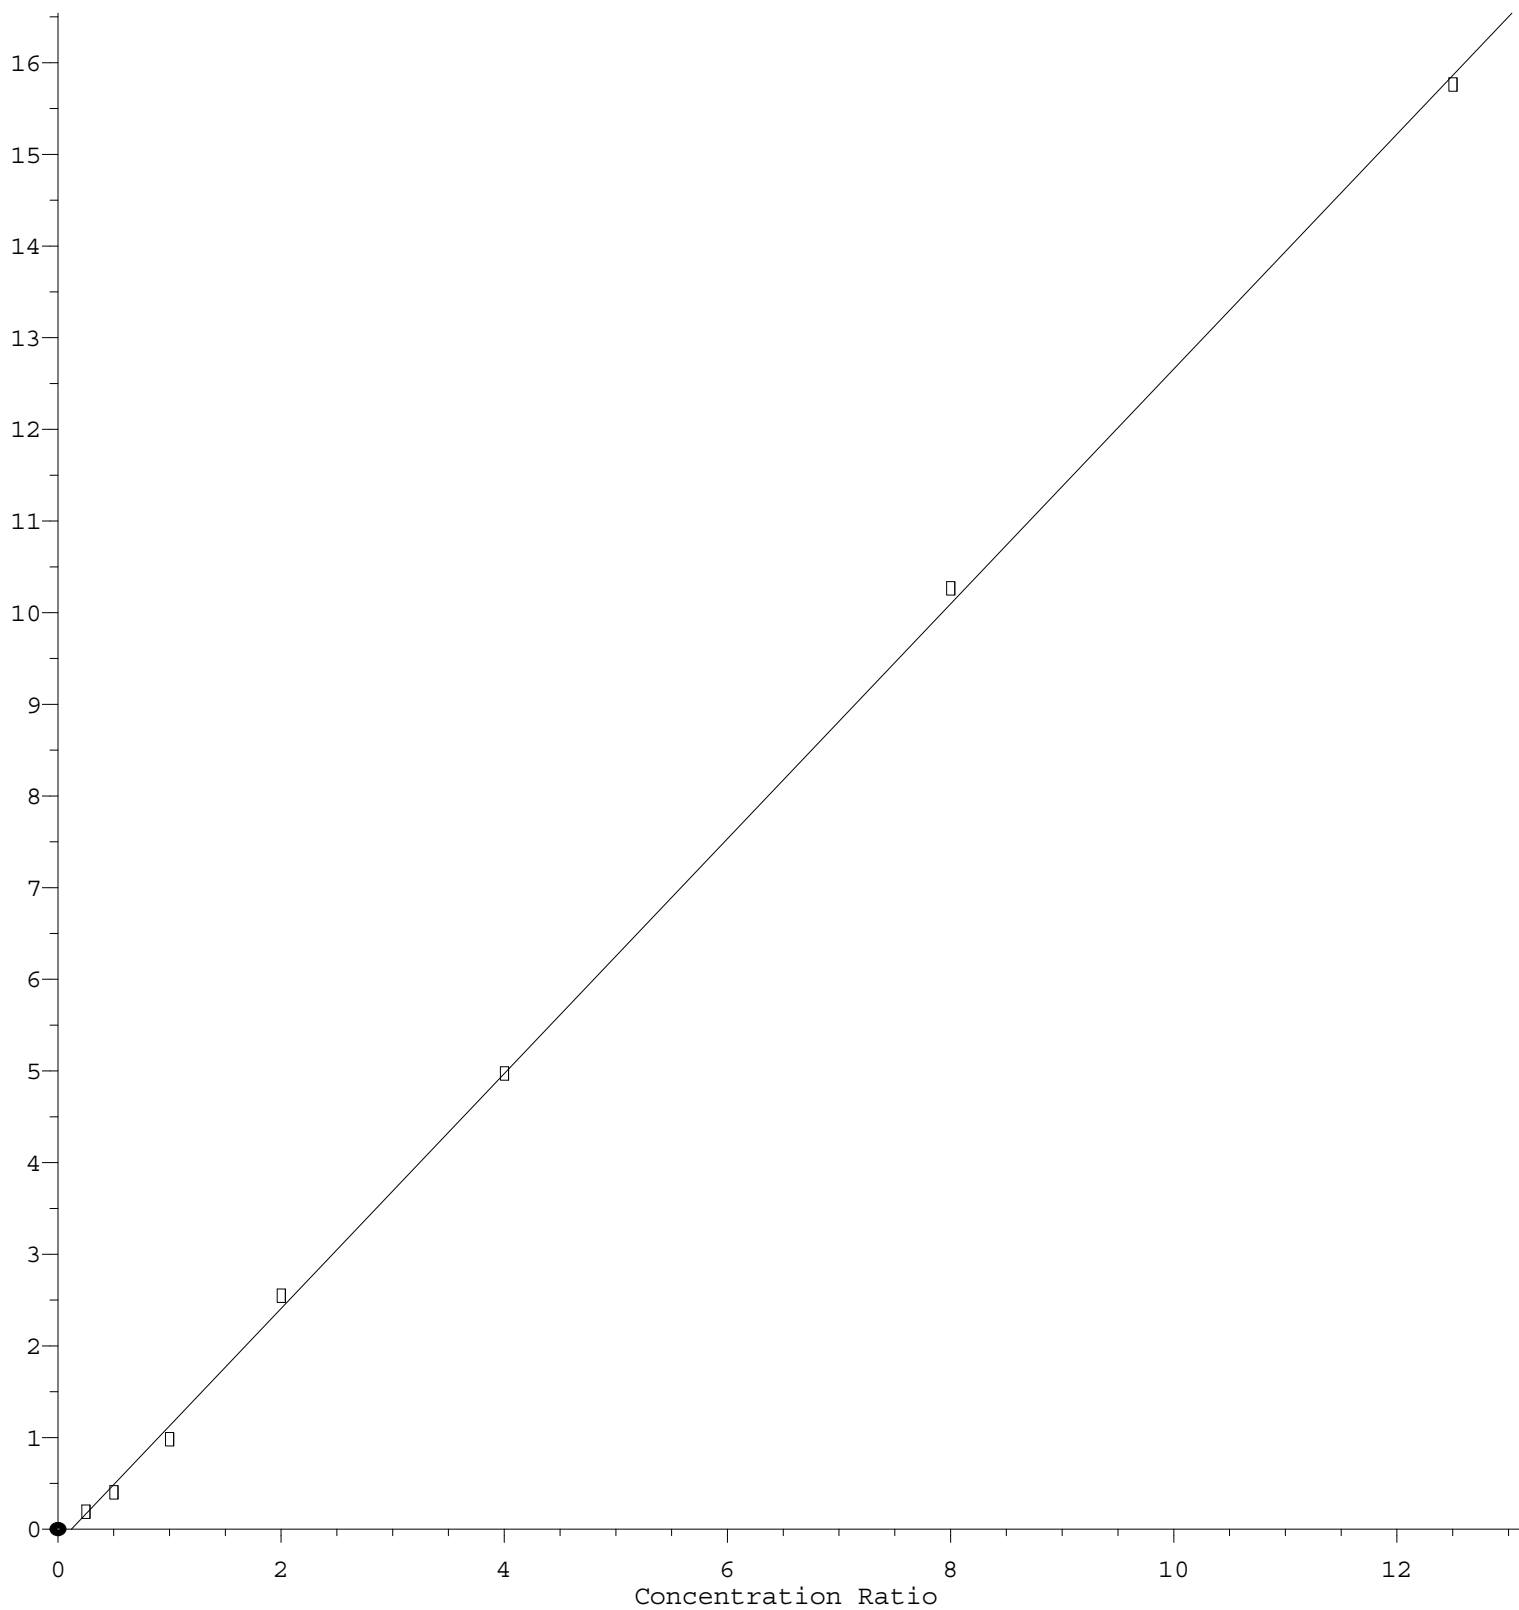

$$\text{Response} = 1.283\text{e}+000 * \text{Amt} - 1.600\text{e}-001$$


Coef of Det (r^2) = 0.999589 Curve Fit: Linear

Method Name: Z:\SVOASRV\HPCHEM1\BNA N\METHODS\8270-SIM-BN121121.M

Calibration Table Last Updated: Sat Dec 11 00:01:30 2021

Indeno(1,2,3-cd)pyrene

Response Ratio

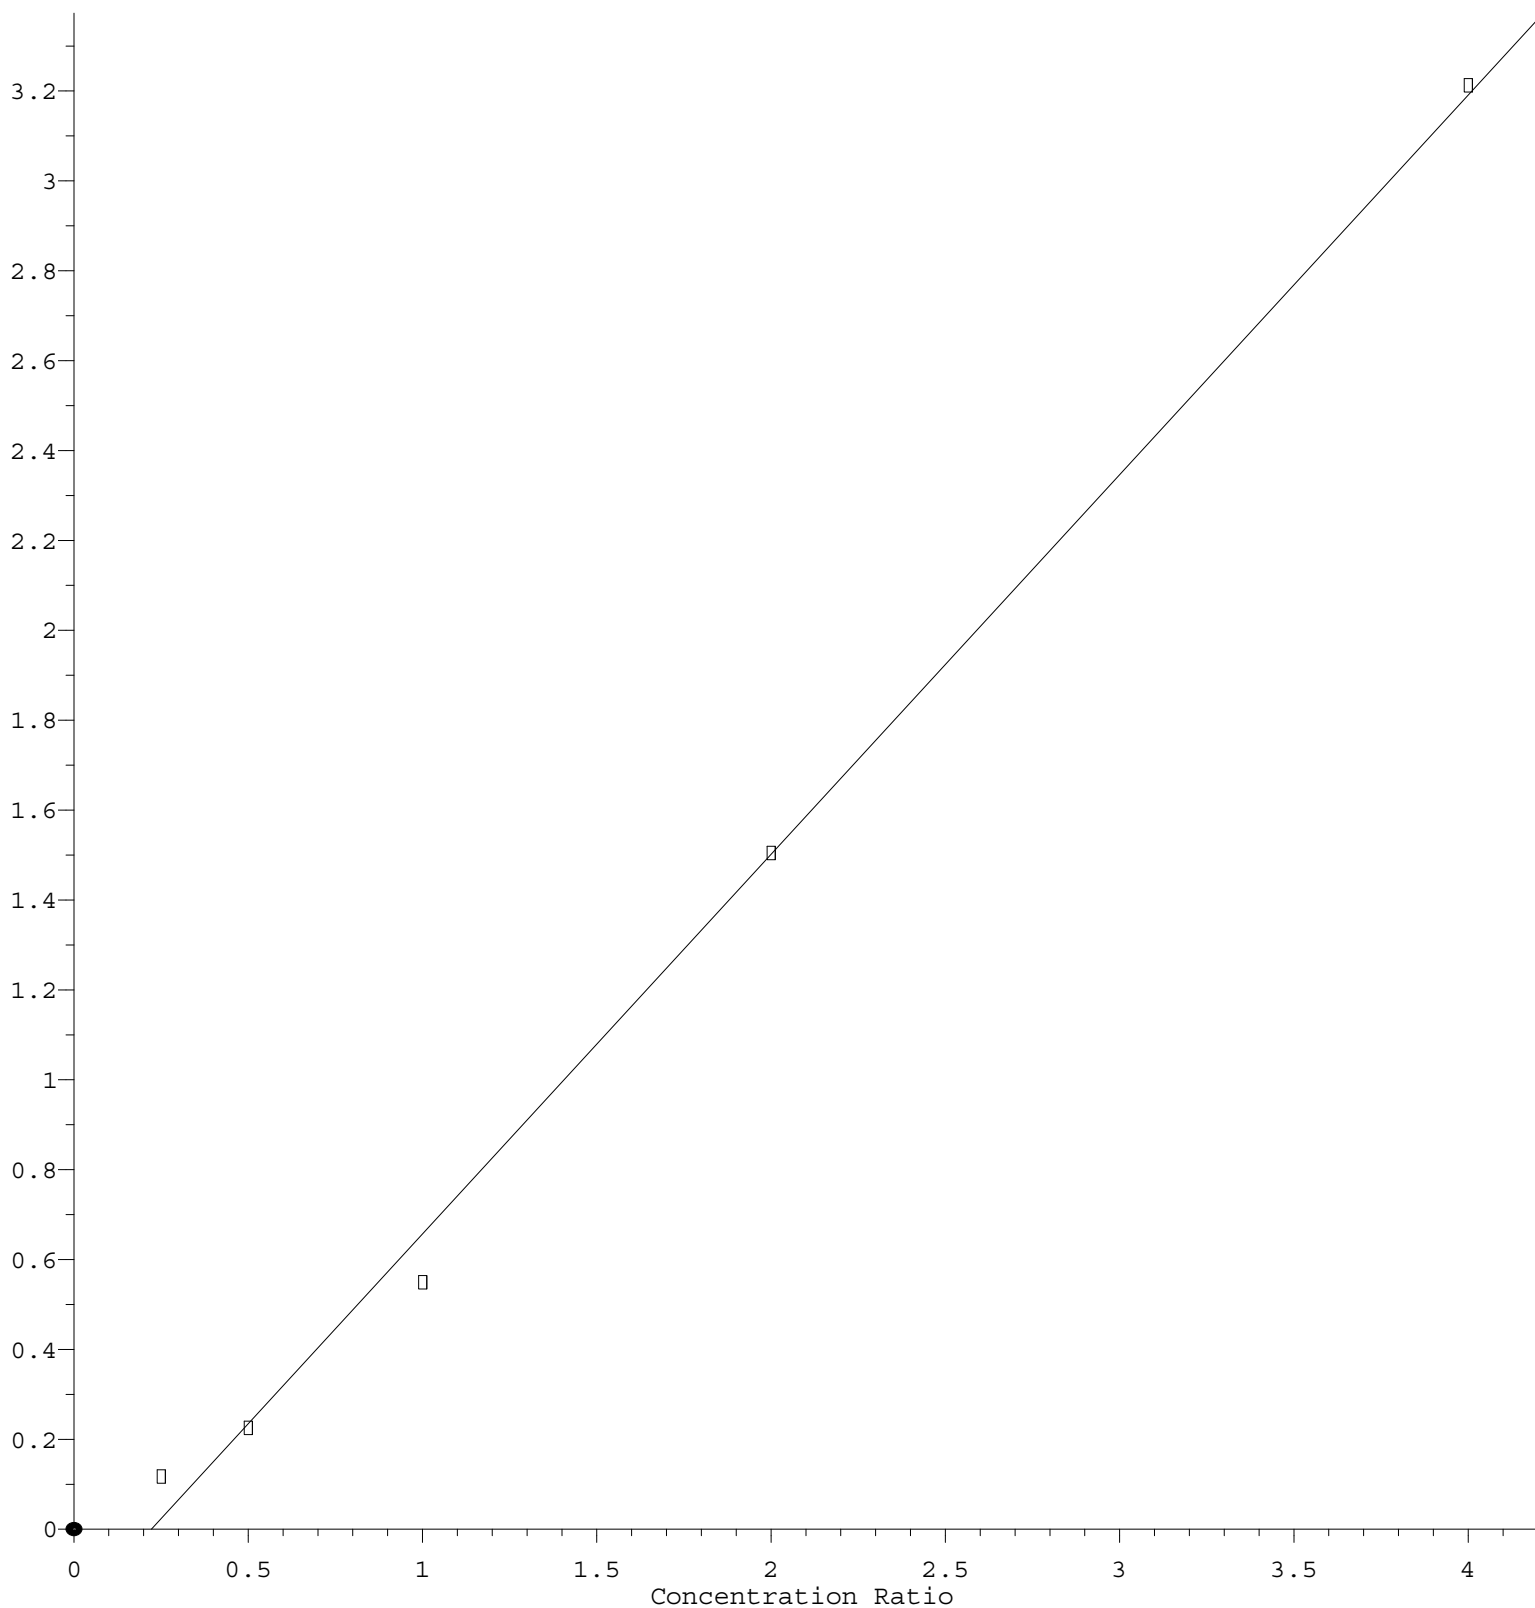

$$\text{Response} = 8.448\text{e-}001 * \text{Amt} - 1.877\text{e-}001$$


Coef of Det (r^2) = 0.996855 Curve Fit: Linear

Method Name: Z:\SVOASRV\HPCHEM1\BNA N\METHODS\8270-SIM-BN121121.M

Calibration Table Last Updated: Sat Dec 11 00:01:30 2021

Dibenzo (a,h) anthracene

Response Ratio

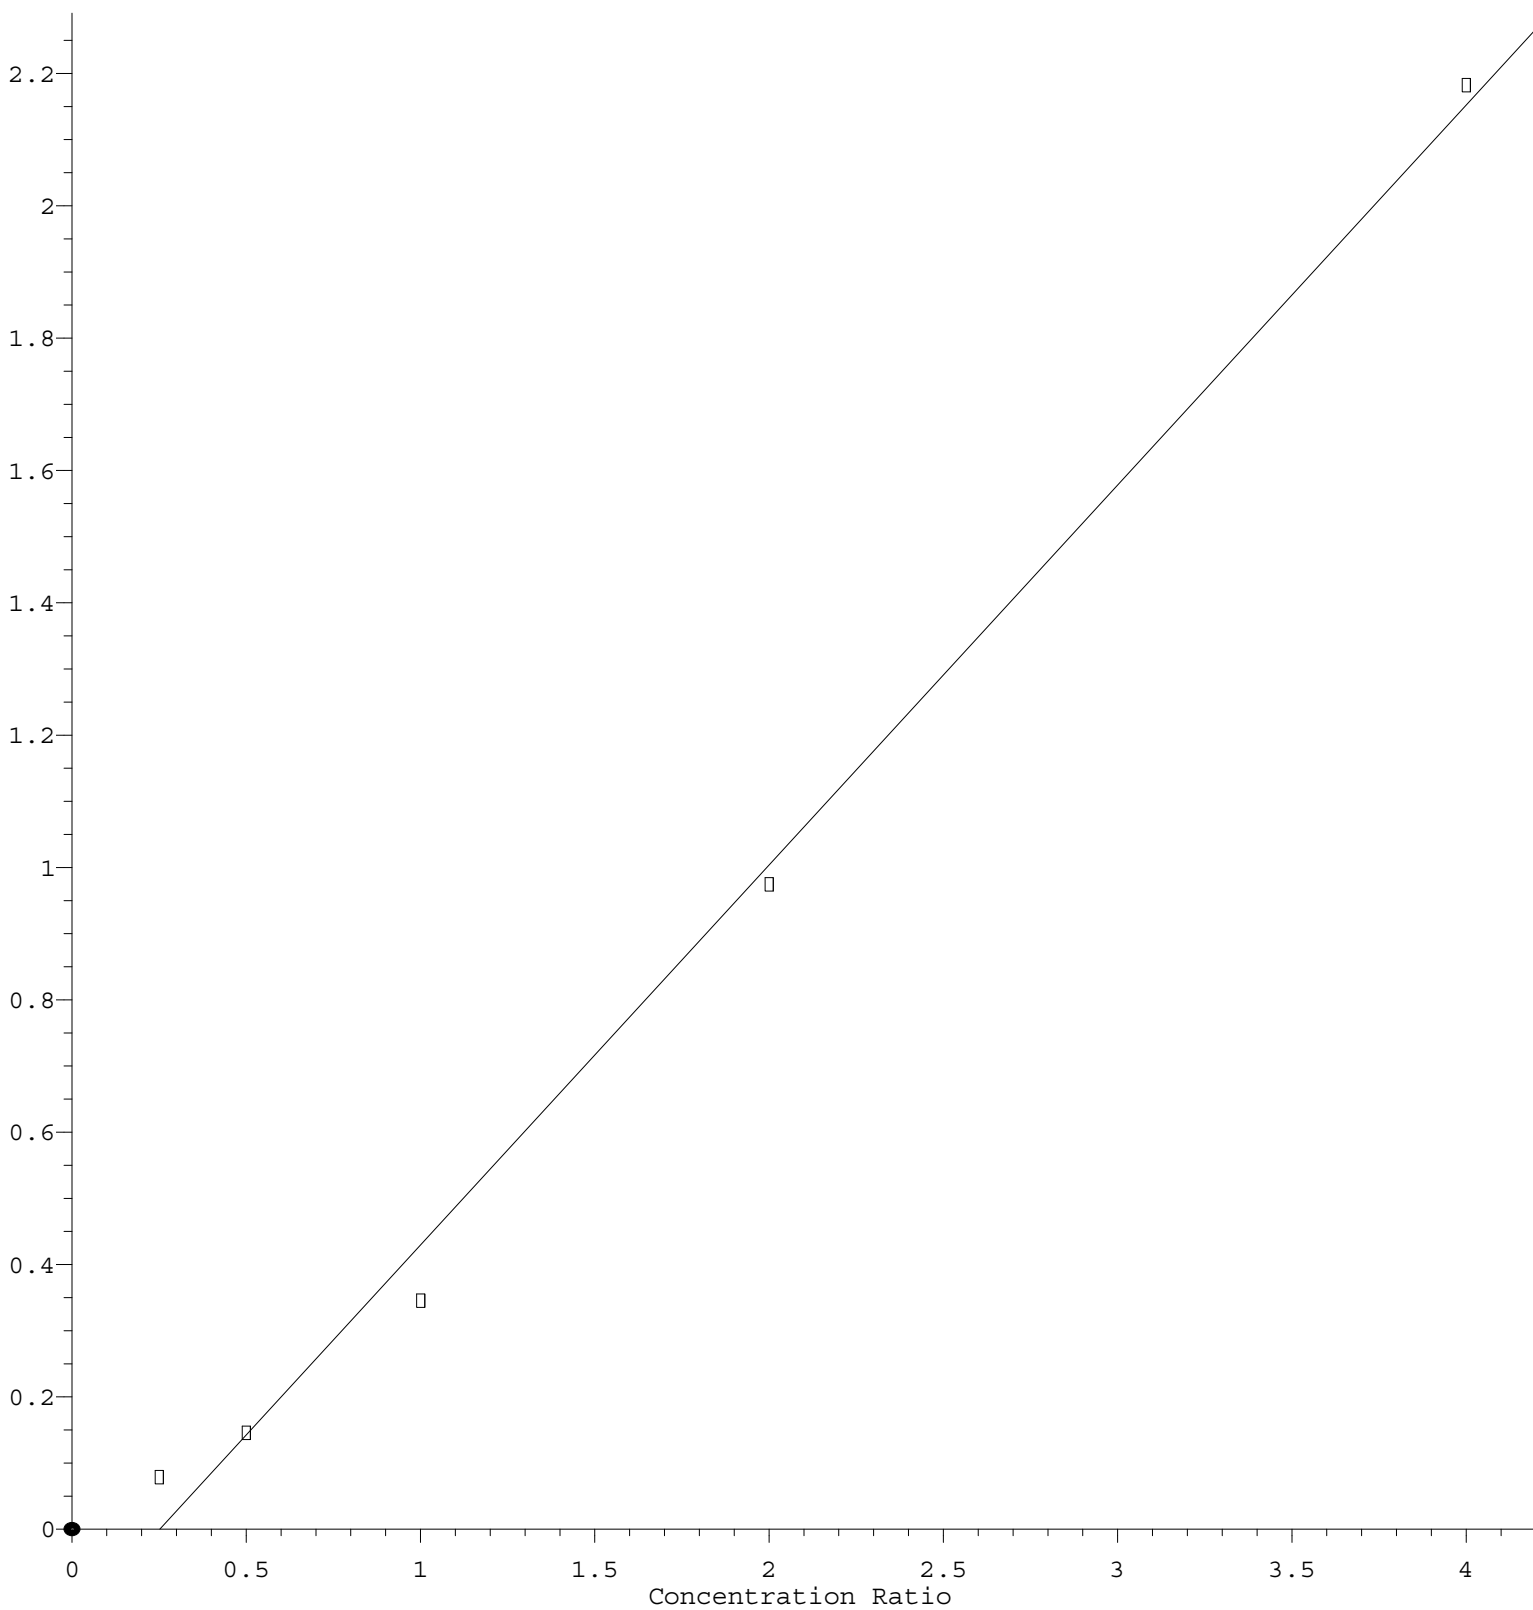


$$\text{Response} = 5.742\text{e-}001 * \text{Amt} - 1.448\text{e-}001$$

Coef of Det (r^2) = 0.995048 Curve Fit: Linear

Method Name: Z:\SVOASRV\HPCHEM1\BNA N\METHODS\8270-SIM-BN121121.M


Calibration Table Last Updated: Sat Dec 11 00:01:30 2021

4,6-Dinitro-2-methylphenol

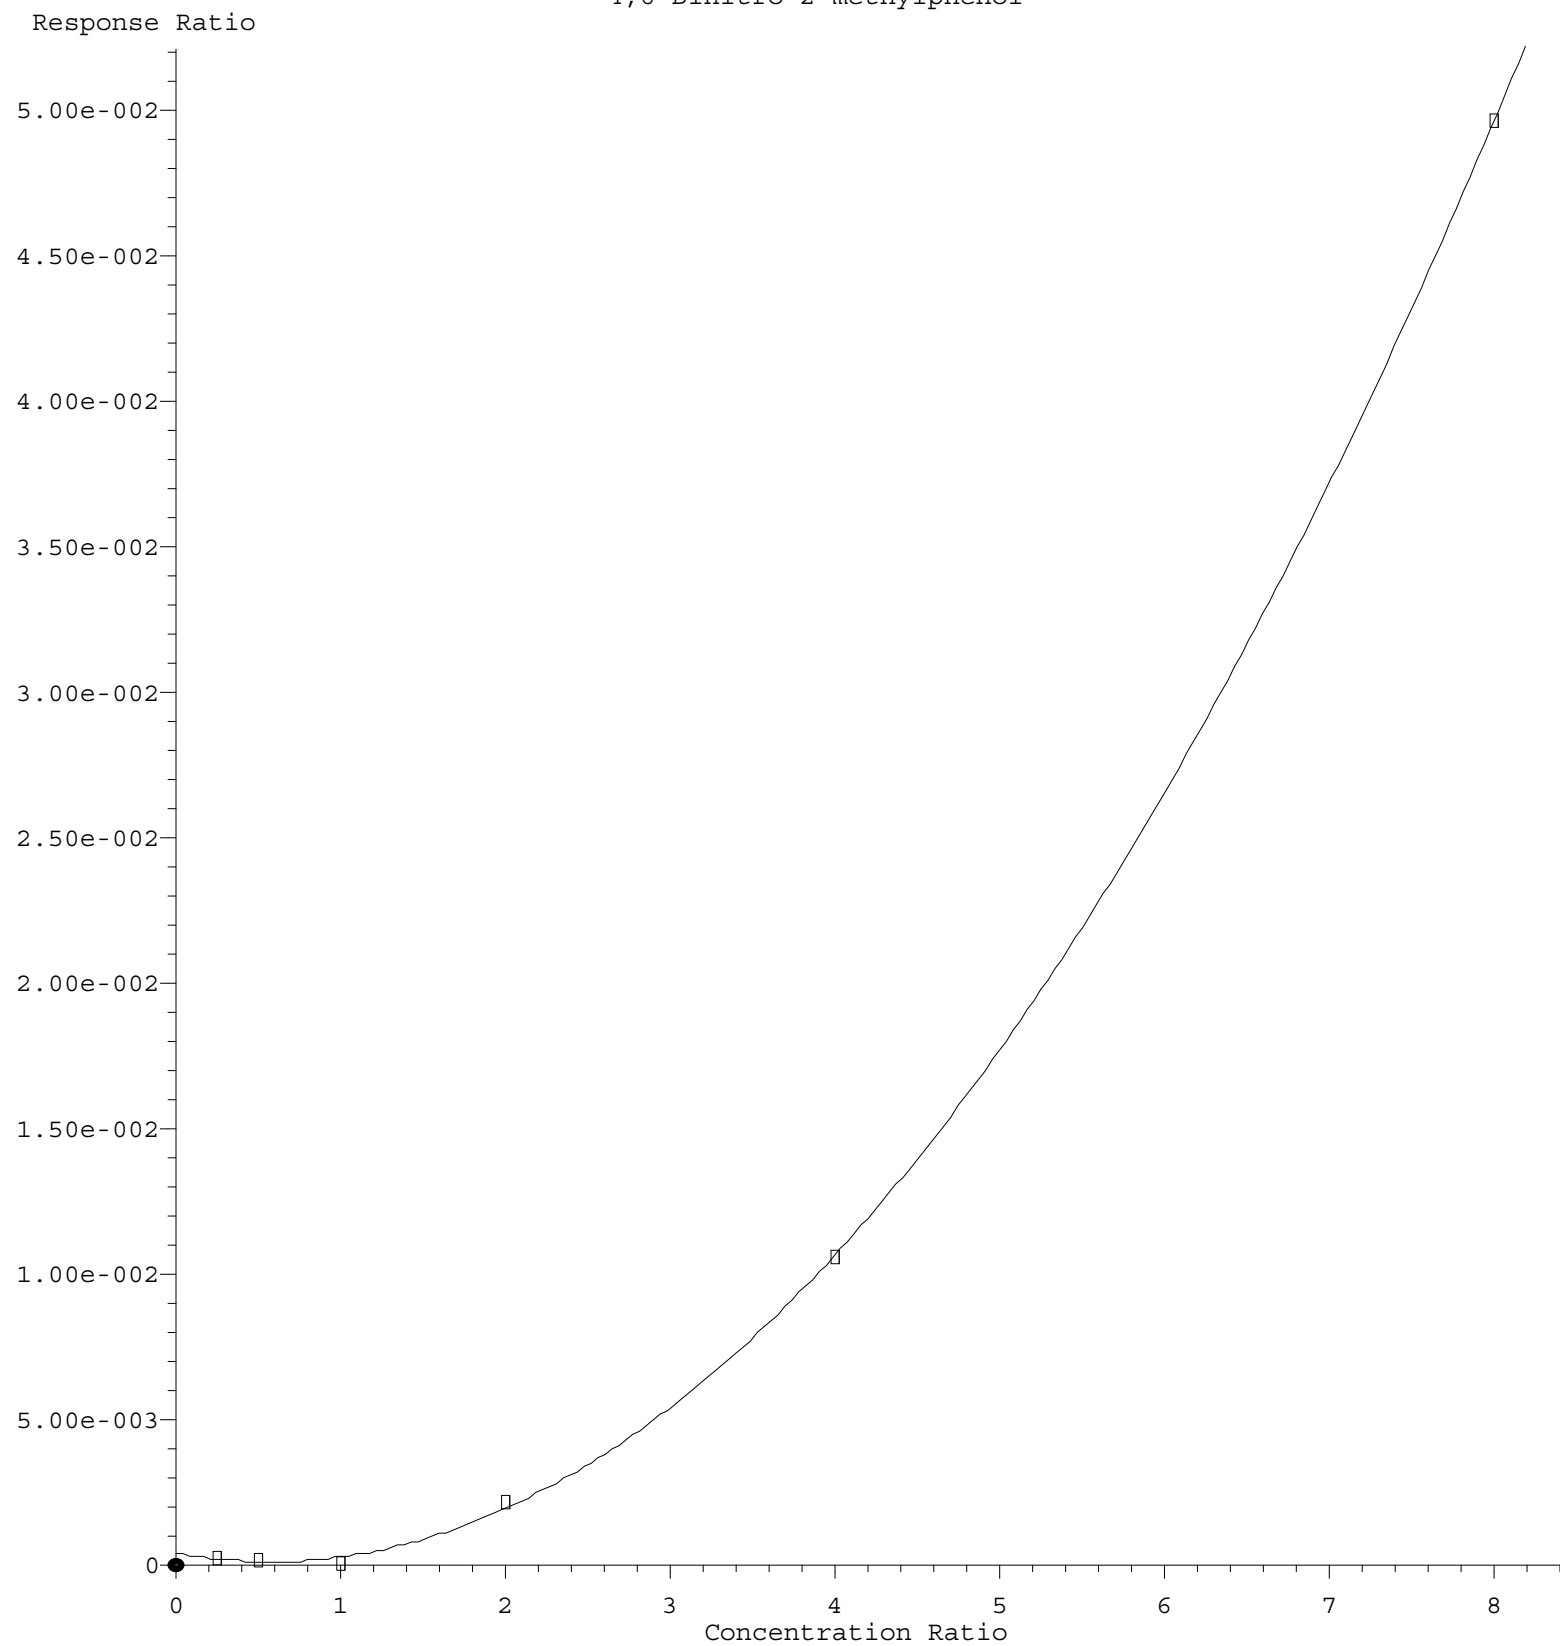

$R = 8.970e-004 A^2 - 1.024e-003 A + 4.096e-004$
 Coef of Det (r^2) = 0.999943 Curve Fit: Quadratic
 Method Name: Z:\SVOASRV\HPCHEM1\BNA N\METHODS\8270-SIM-BN121121.M
 Calibration Table Last Updated: Sat Dec 11 00:01:30 2021

Pentachlorophenol

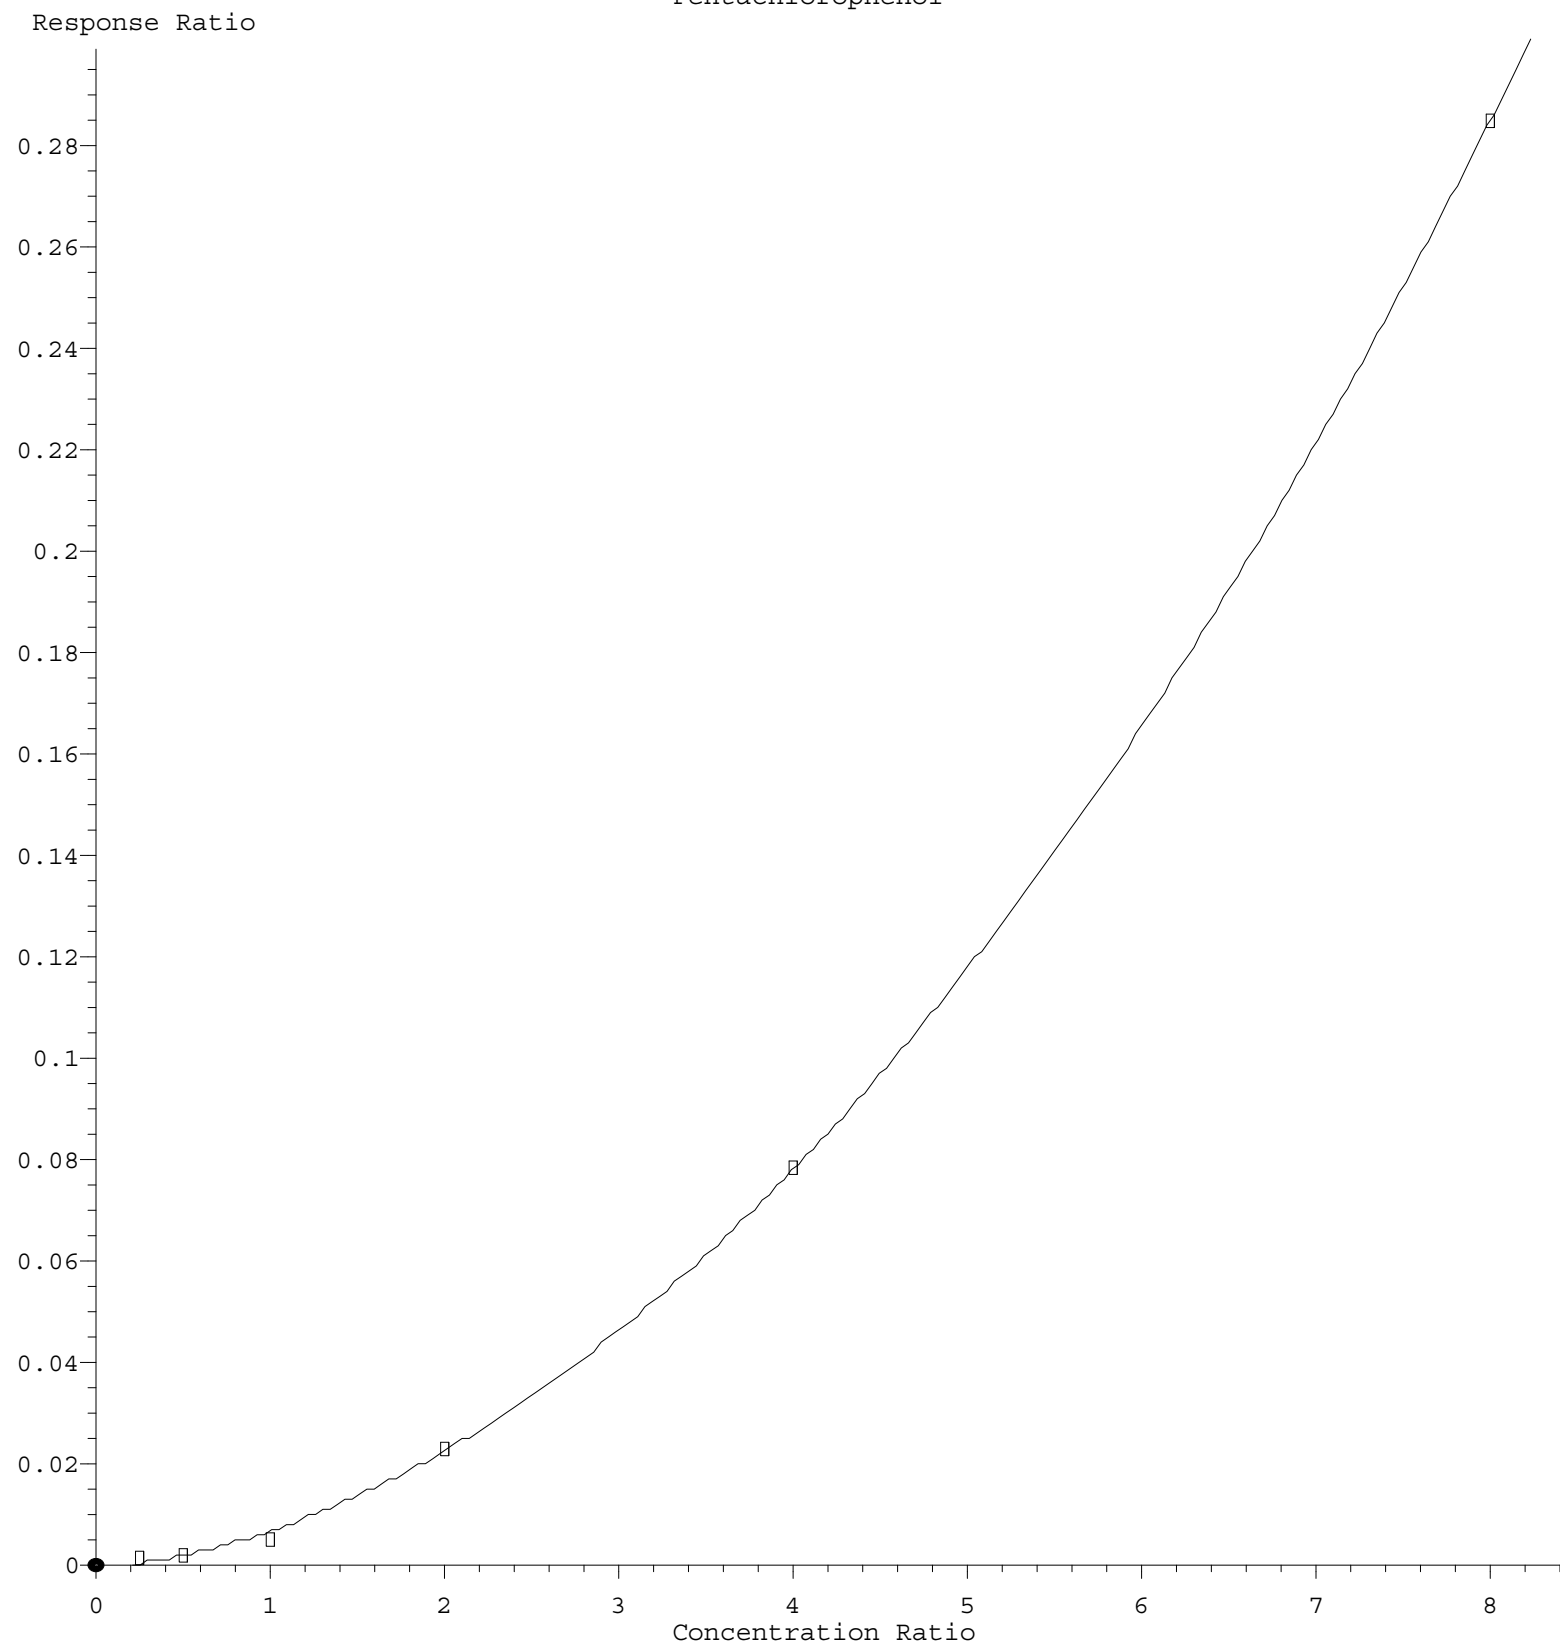

$R = 4.000e-003 A^2 + 3.737e-003 A - 9.169e-004$
 Coef of Det (r^2) = 0.999922 Curve Fit: Quadratic
 Method Name: Z:\SVOASRV\HPCHEM1\BNA N\METHODS\8270-SIM-BN121121.M
 Calibration Table Last Updated: Sat Dec 11 00:01:30 2021