
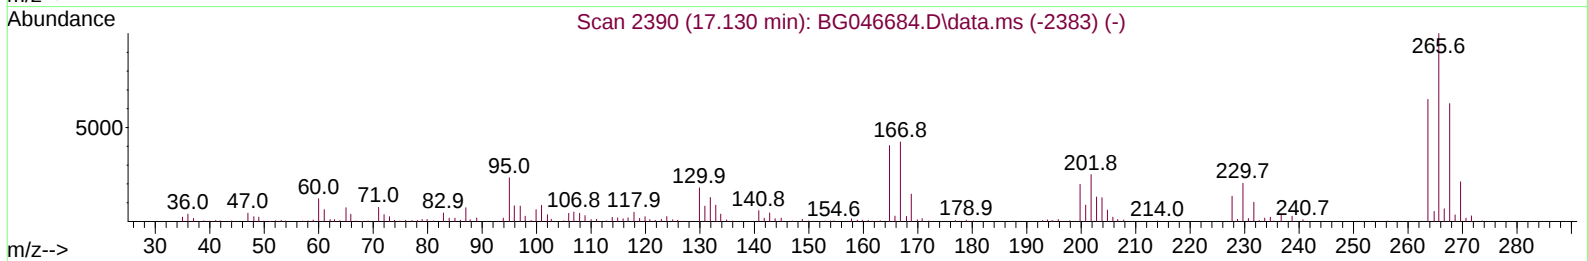
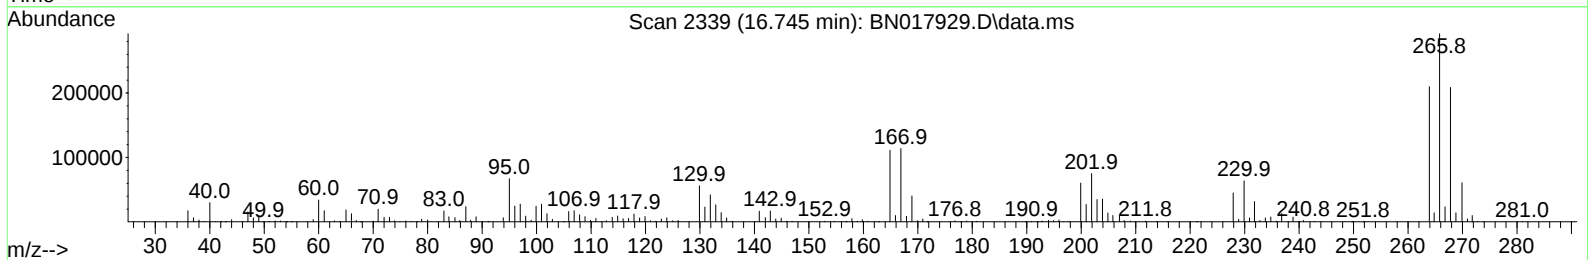


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121121\
 Data File : BN017929.D
 Acq On : 12 Dec 2021 07:05
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 53 Sample Multiplier: 1

Quant Time: Dec 13 03:16:47 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Dec 13 03:14:02 2021
 Response via : Initial Calibration

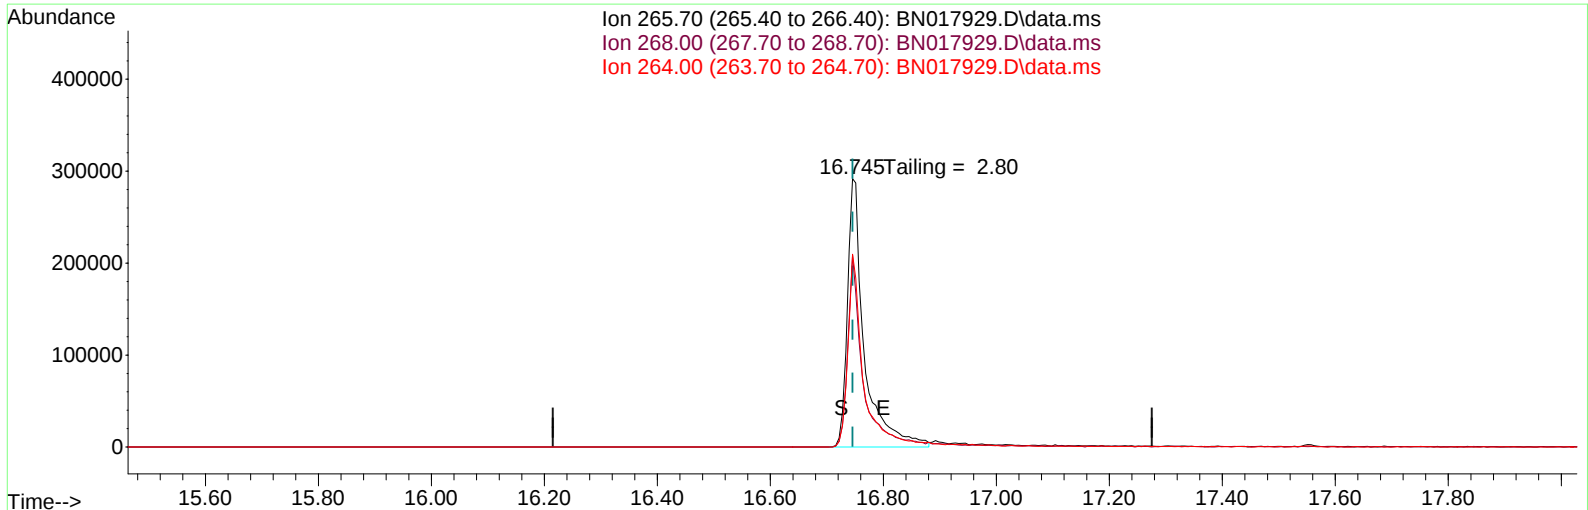

TIC: BN017929.D\data.ms

(70) Pentachlorophenol (C)




16.745min (+ 0.000) 11603.66 ng

response 610575

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	71.48
264.00	61.60	71.85
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121121\
Data File : BN017929.D
Acq On : 12 Dec 2021 07:05
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 53 Sample Multiplier: 1

Quant Time: Dec 13 03:16:47 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 13 03:14:02 2021
Response via : Initial Calibration

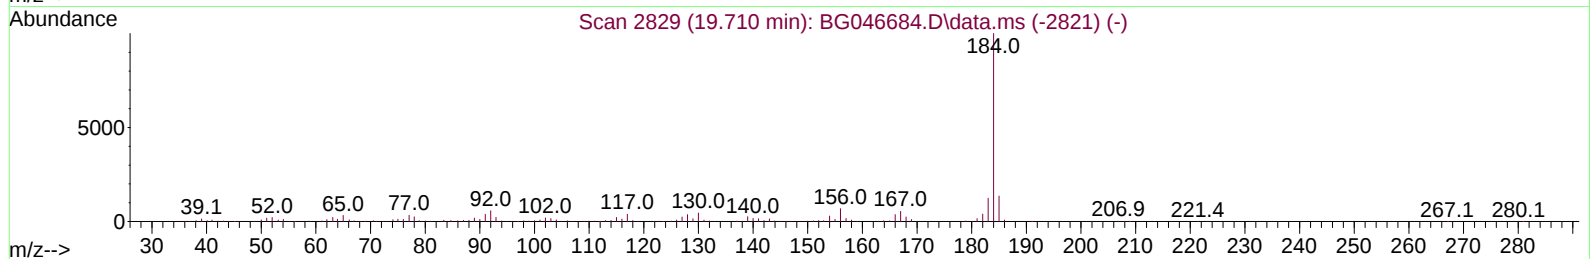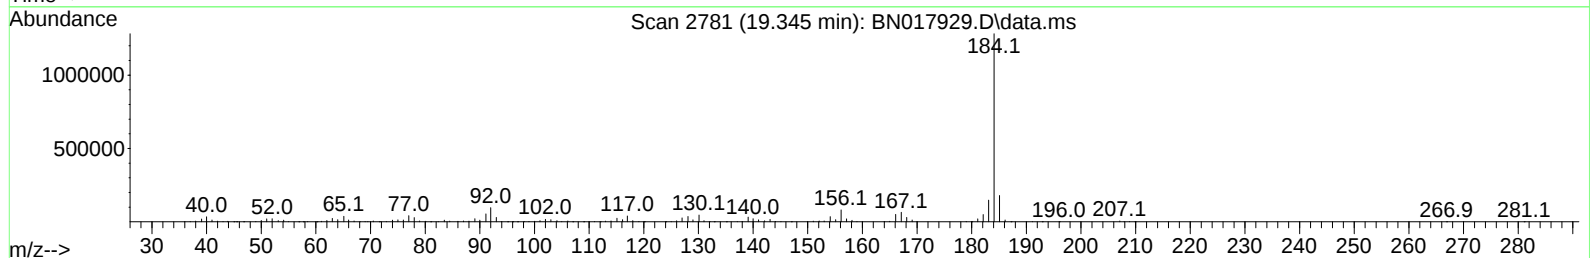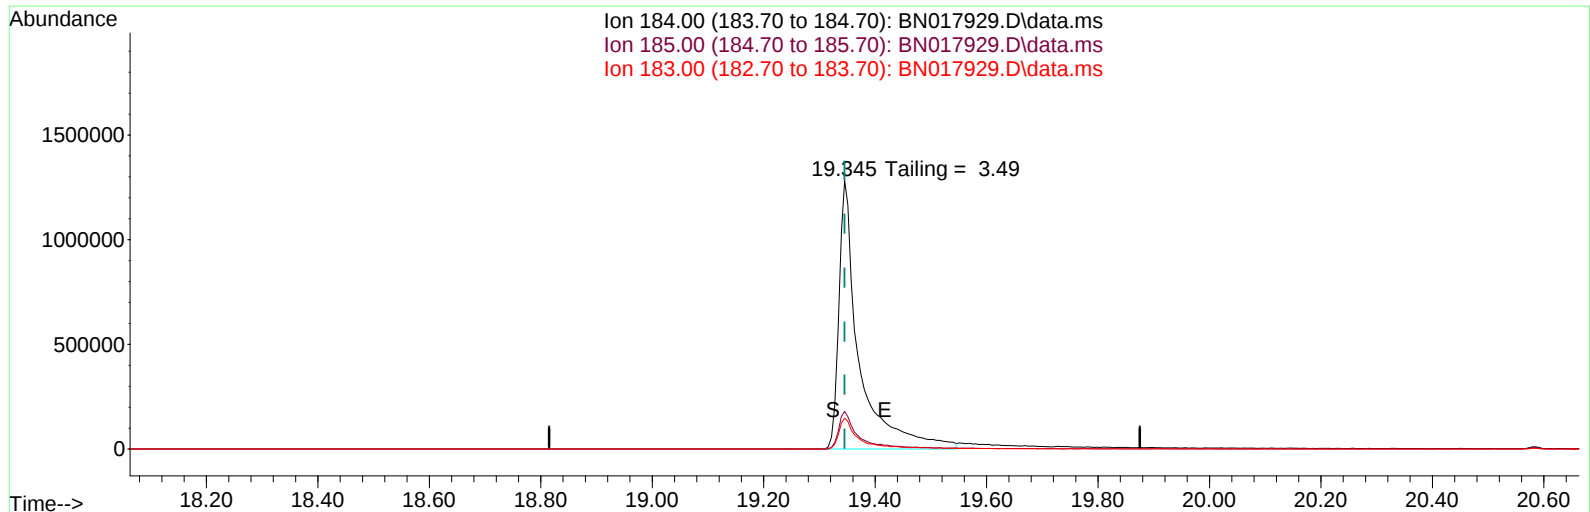

TIC: BN017929.D\data.ms

(77) Benzidine**19.345min (+ 0.000) 0.00 ng****response 3398259**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.02
183.00	13.20	11.53
0.00	0.00	0.00