
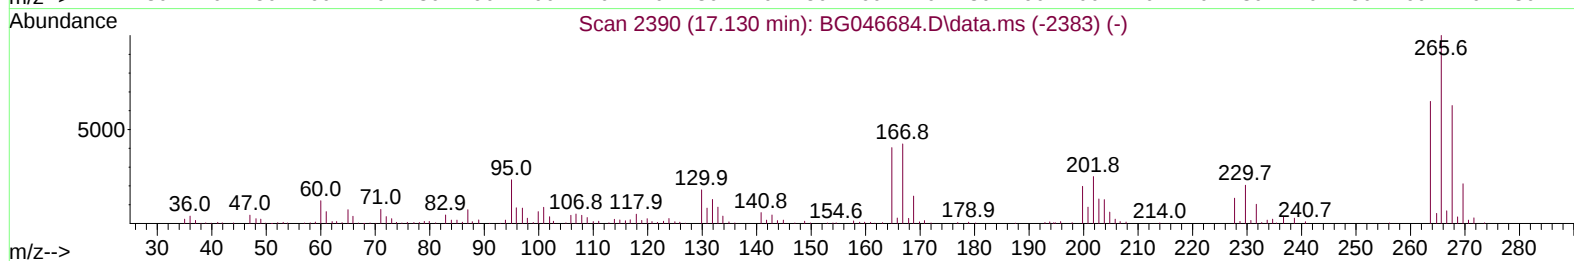
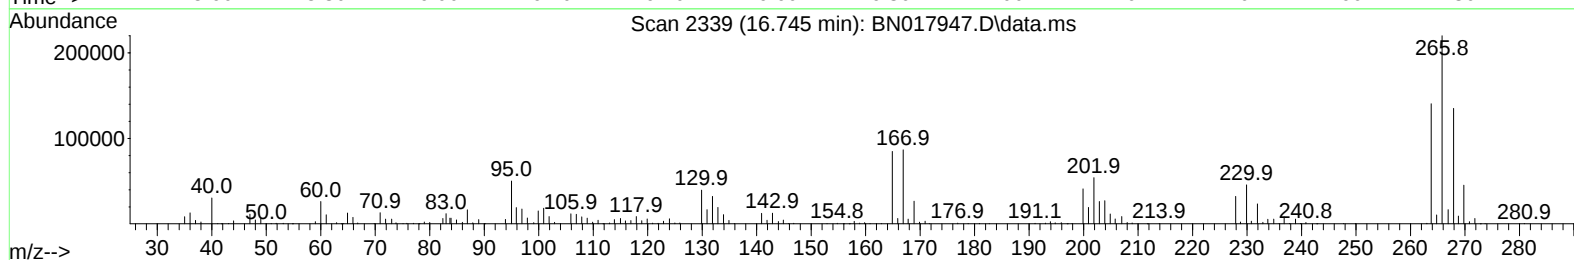


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121121\
Data File : BN017947.D
Acq On : 12 Dec 2021 20:17
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 72 Sample Multiplier: 1

Quant Time: Dec 13 03:14:07 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 13 03:14:02 2021
Response via : Initial Calibration

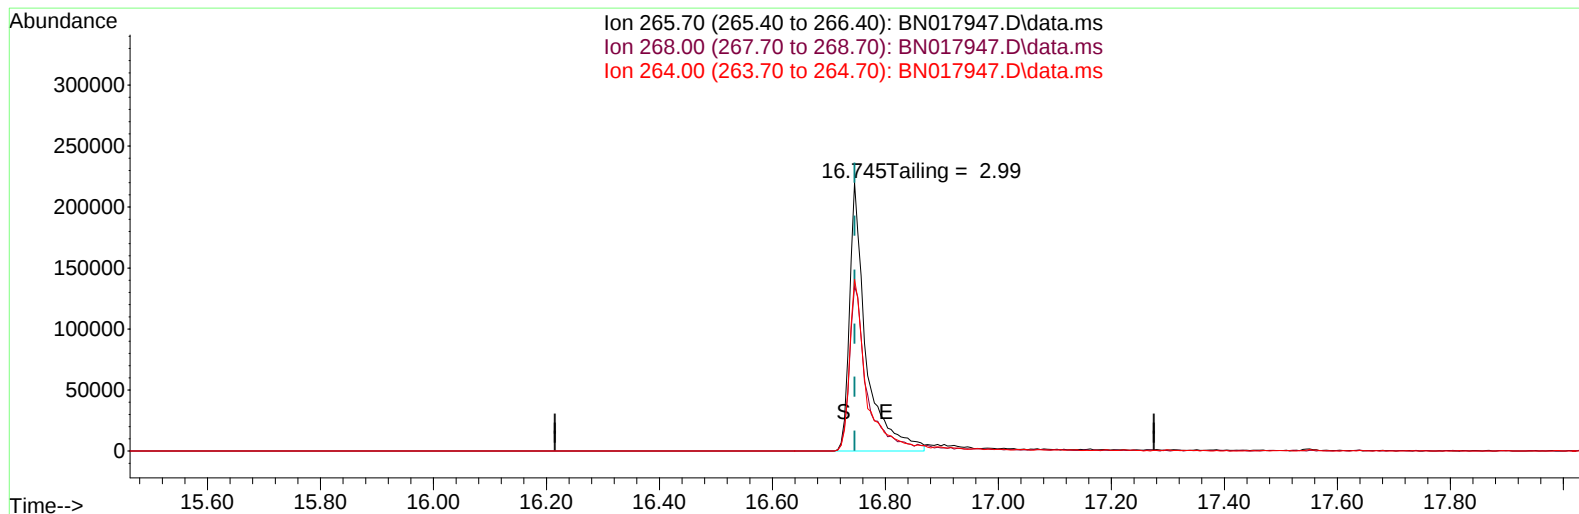

TIC: BN017947.D\data.ms

(70) Pentachlorophenol (C)




16.745min (0.000) 14856.63 ng

response 455638

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	61.40
264.00	61.60	63.90
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121121\
 Data File : BN017947.D
 Acq On : 12 Dec 2021 20:17
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 72 Sample Multiplier: 1

Quant Time: Dec 13 03:14:07 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Dec 13 03:14:02 2021
 Response via : Initial Calibration

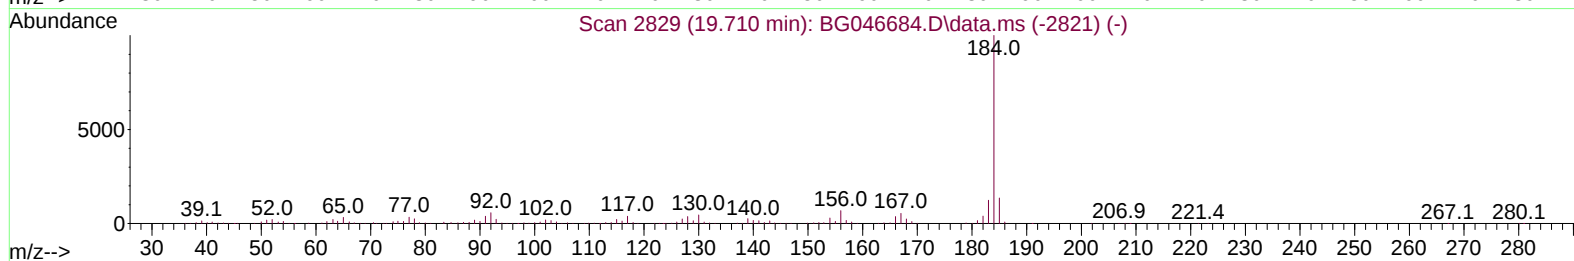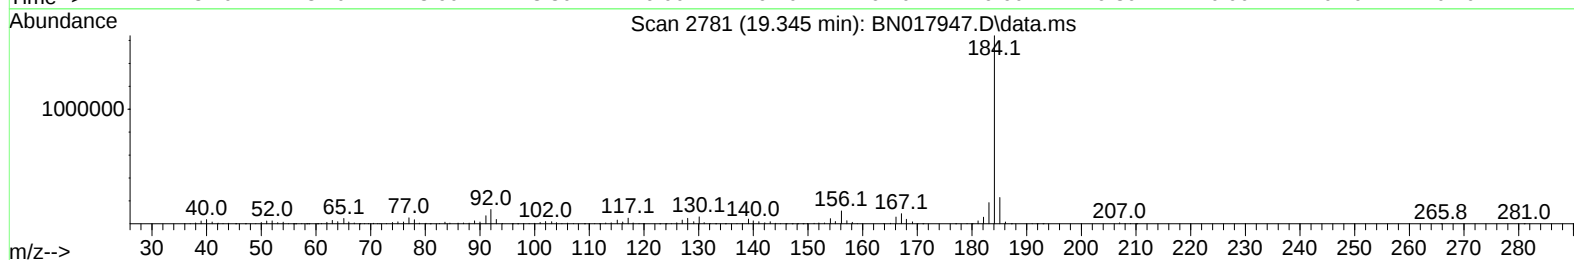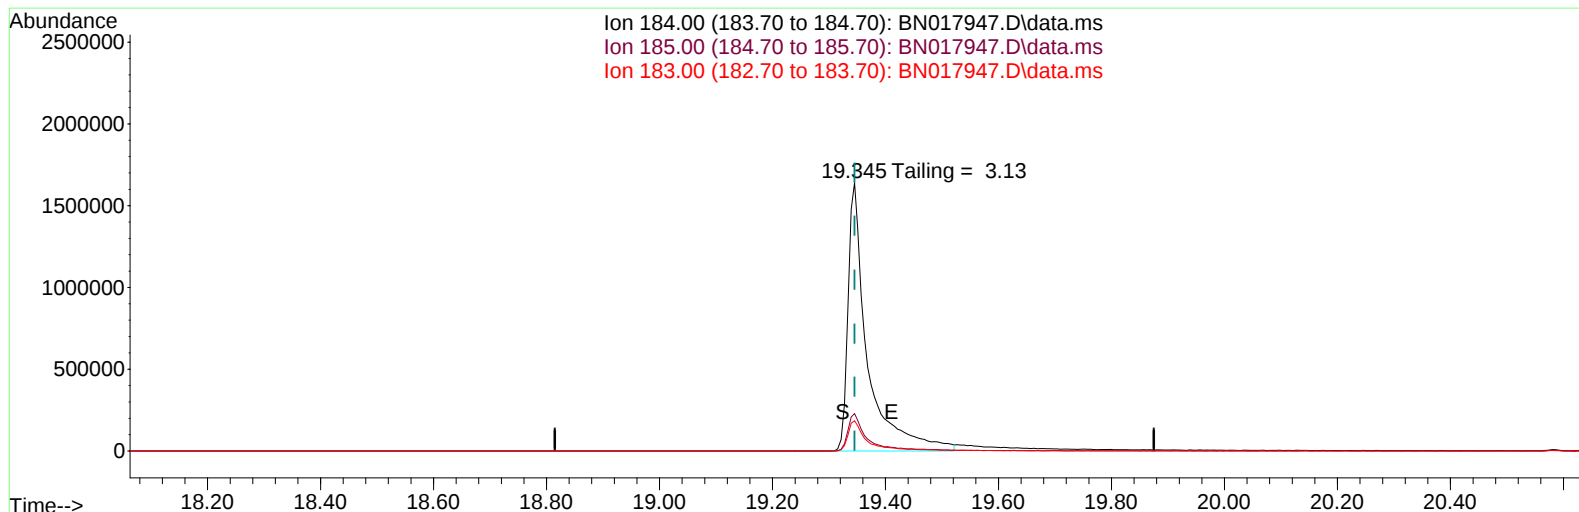

TIC: BN017947.D\data.ms

(77) Benzidine**19.345min (0.000) 0.00 ng****response 4108089**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.95
183.00	13.20	11.28
0.00	0.00	0.00