

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121121\
 Data File : BN017908.D
 Acq On : 11 Dec 2021 15:58
 Operator : CG/JU
 Sample : M4957-09
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 MW179D-20211206

Quant Time: Dec 11 21:30:52 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN121121.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Dec 11 00:01:30 2021
 Response via : Initial Calibration

Manual Integrations
 APPROVED

Reviewed By : Christian Giraldo 12/15/2021
 Supervised By : Yogesh Patel 12/16/2021

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.715	152	24622	0.400	ng	0.00
7) Naphthalene-d8	10.494	136	103116	0.400	ng	0.00
13) Acenaphthene-d10	14.335	164	69754	0.400	ng	0.00
19) Phenanthrene-d10	17.080	188	136877	0.400	ng	#-0.01
29) Chrysene-d12	21.293	240	97224	0.400	ng	# 0.00
35) Perylene-d12	23.589	264	77027	0.400	ng	0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.336	112	5453	0.107	ng	0.00
5) Phenol-d6	6.903	99	2715	0.054	ng	0.00
8) Nitrobenzene-d5	8.859	82	18369	0.273	ng	0.00
11) 2-Methylnaphthalene-d10	12.085	152	46517	0.257	ng	0.00
14) 2,4,6-Tribromophenol	15.844	330	4996	0.464	ng	0.00
15) 2-Fluorobiphenyl	12.964	172	73178	0.298	ng	0.00
27) Fluoranthene-d10	19.124	212	137579	0.310	ng	0.00
31) Terphenyl-d14	19.730	244	108865	0.454	ng	0.00
Target Compounds						Qvalue
2) 1,4-Dioxane	3.270	88	1134m	0.152	ng	
6) bis(2-Chloroethyl)ether	7.143	93	1420	0.023	ng	# 1
9) Naphthalene	10.545	128	9039	0.035	ng	97
34) Bis(2-ethylhexyl)phtha...	21.208	149	1045668	10.018	ng	98
36) Indeno(1,2,3-cd)pyrene	25.985	276	1255	0.097	ng	# 60
40) Dibenzo(a,h)anthracene	25.999	278	975m	0.110	ng	

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121121\
Data File : BN017908.D
Acq On : 11 Dec 2021 15:58
Operator : CG/JU
Sample : M4957-09
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
MW179D-20211206

Manual Integrations
APPROVED

Reviewed By : Christian Giraldo 12/15/2021
Supervised By : Yogesh Patel 12/16/2021


Quant Time: Dec 11 21:30:52 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN121121.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Dec 11 00:01:30 2021
Response via : Initial Calibration

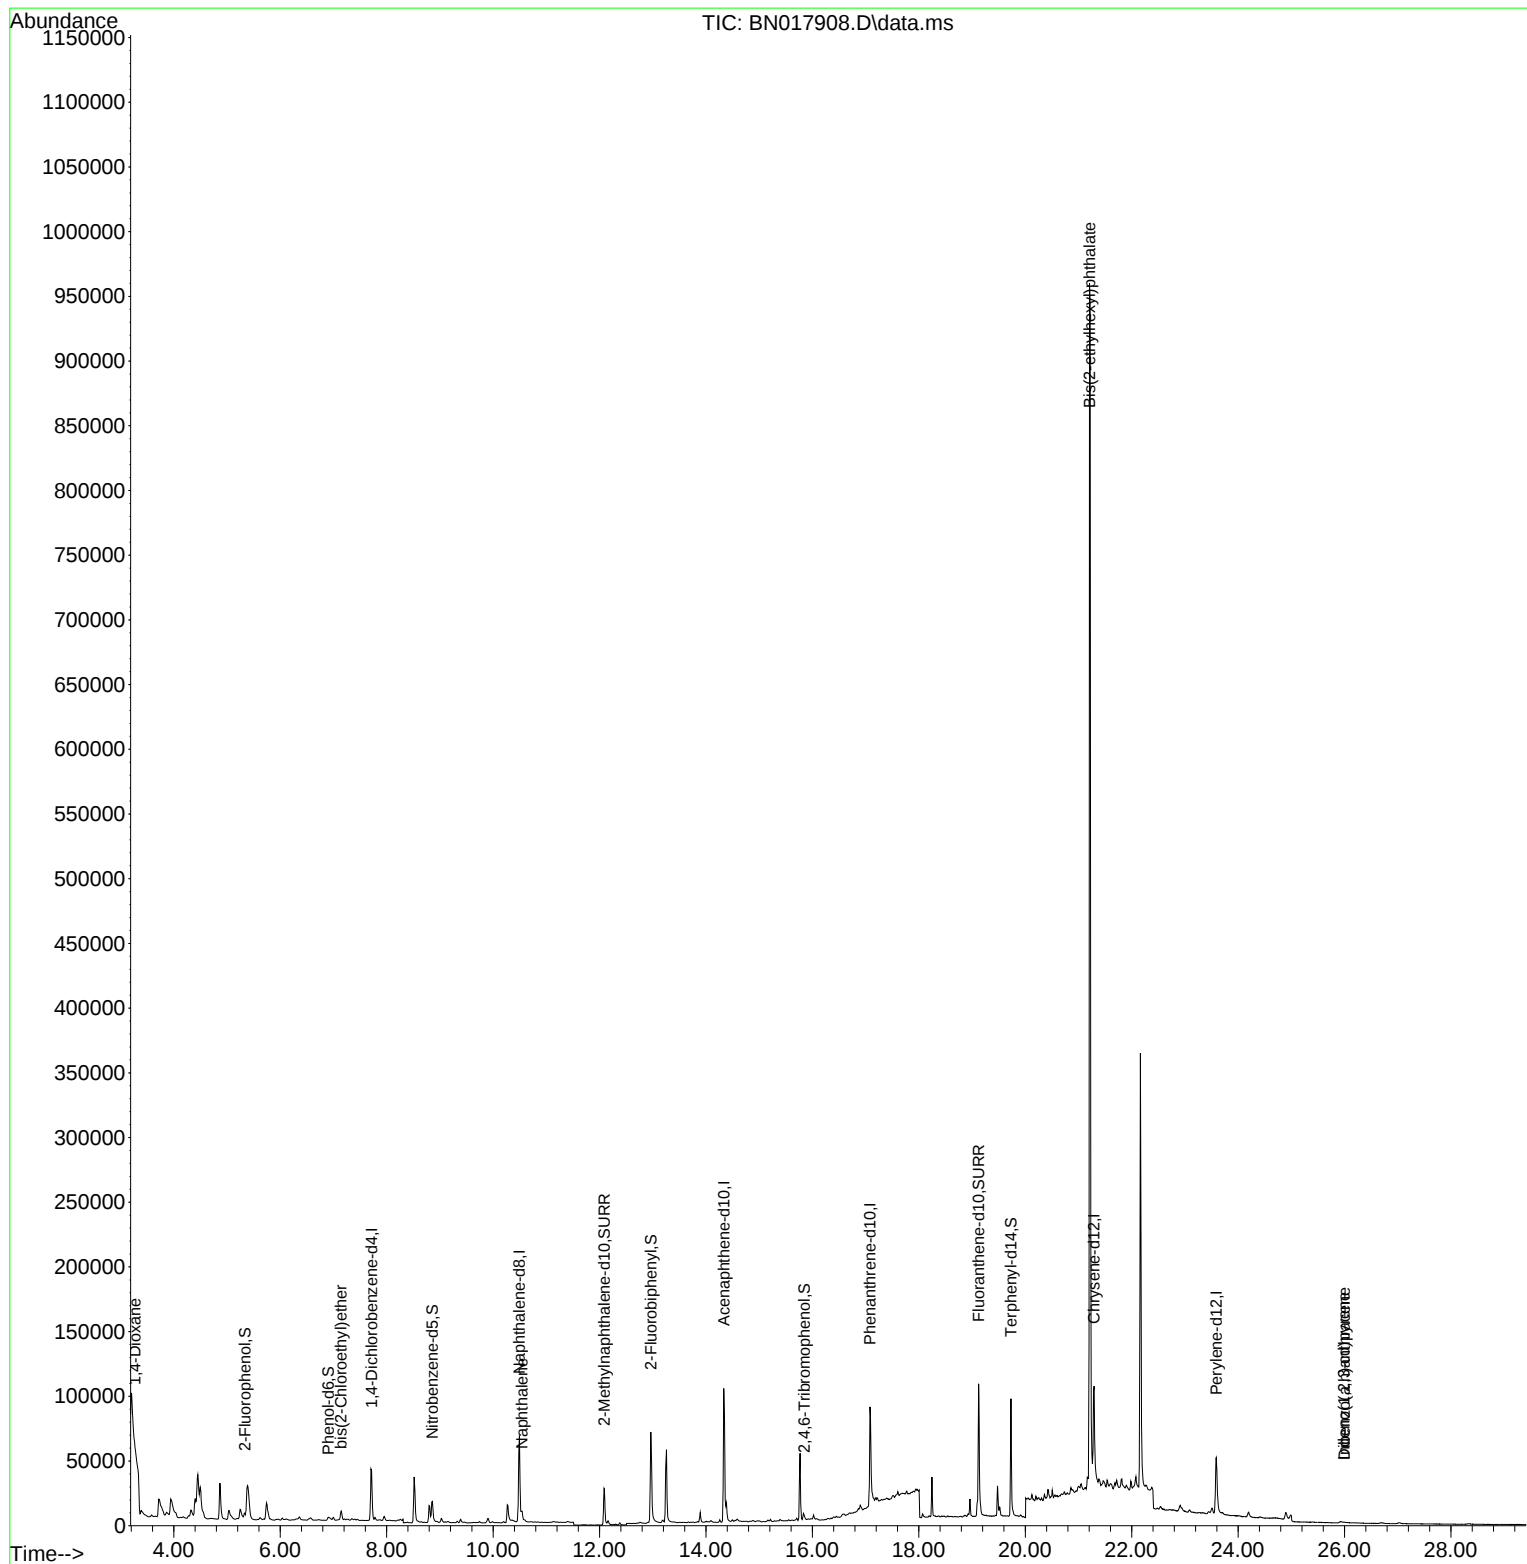



#1
 1,4-Dichlorobenzene-d4
 Concen: 0.400 ng
 RT: 7.715 min Scan# 492
 Delta R.T. -0.000 min
 Lab File: BN017908.D
 Acq: 11 Dec 2021 15:58




Instrument :
 BNA_N
 ClientSampleId :
 MW179D-20211206

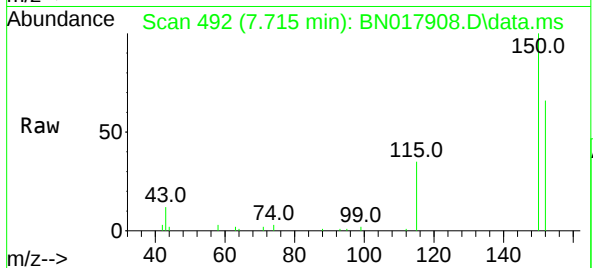


Tgt Ion:152 Resp: 2462
 Ion Ratio Lower Upper
 152 100
 150 151.0 121.9 182.9
 115 53.5 44.1 66.1

Manual Integrations
 APPROVED



Reviewed By :Christian Giraldo 12/15/2021
 Supervised By :Yogesh Patel 12/16/2021

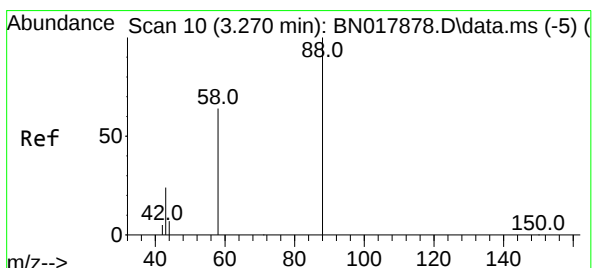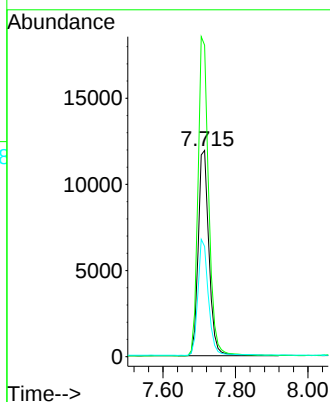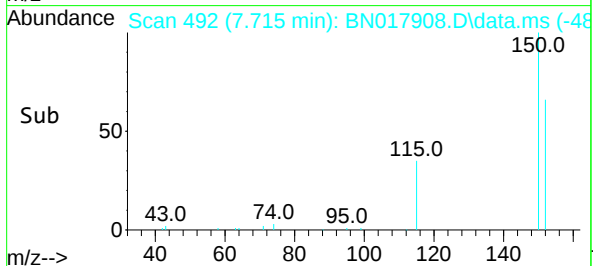


#2
 1,4-Dioxane
 Concen: 0.152 ng m
 RT: 3.270 min Scan# 10
 Delta R.T. 0.000 min
 Lab File: BN017908.D
 Acq: 11 Dec 2021 15:58

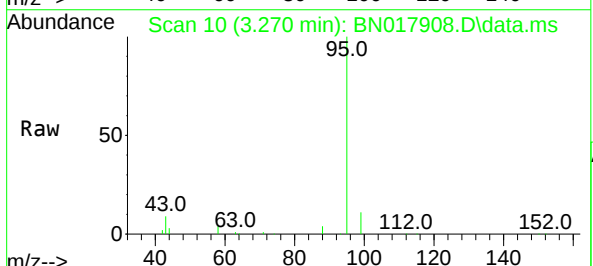

Tgt Ion: 88 Resp: 1134
 Ion Ratio Lower Upper
 88 100
 43 45.2 28.0 42.0#
 58 118.9 65.4 98.0#

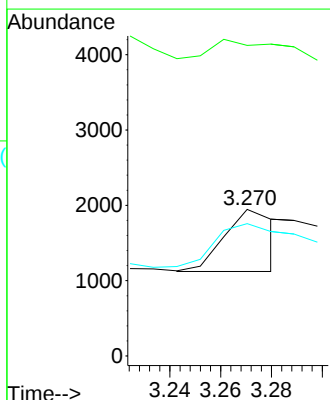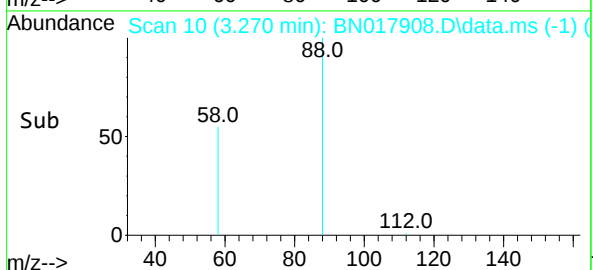







#4
2-Fluorophenol
Concen: 0.107 ng
RT: 5.336 min Scan# 211
Delta R.T. 0.009 min
Lab File: BN017908.D
Acq: 11 Dec 2021 15:58

Instrument :
BNA_N
ClientSampleId :
MW179D-20211206

Tgt Ion:112 Resp: 545
Ion Ratio Lower Upper
112 100
64 37.0 49.0 73.4
63 0.0 26.2 39.2




Manual Integrations
APPROVED


Reviewed By :Christian Giraldo 12/15/2021
Supervised By :Yogesh Patel 12/16/2021

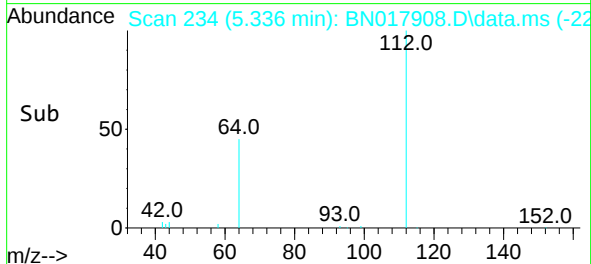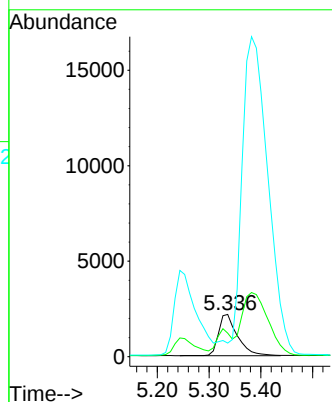

#5
Phenol-d6
Concen: 0.054 ng
RT: 6.903 min Scan# 404
Delta R.T. 0.009 min
Lab File: BN017908.D
Acq: 11 Dec 2021 15:58


Tgt Ion: 99 Resp: 2715
Ion Ratio Lower Upper
99 100
42 23.1 17.0 25.4
71 42.7 28.0 42.0

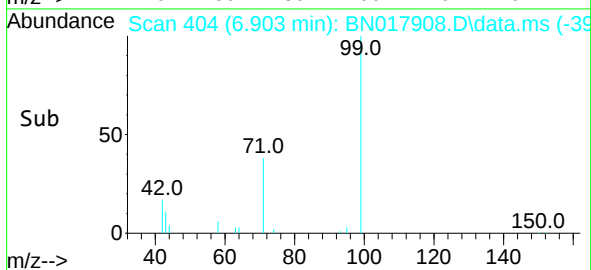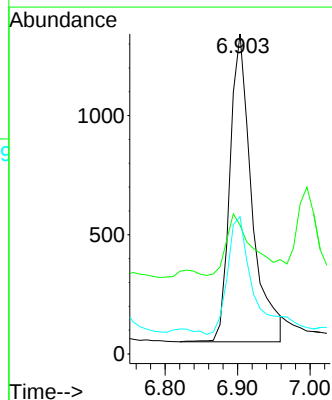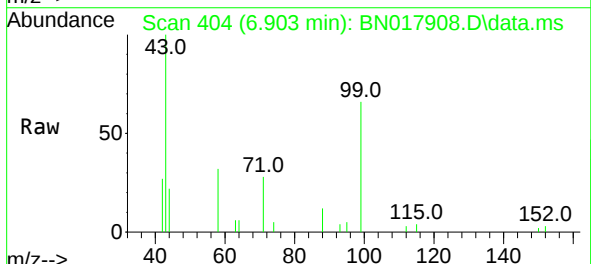



#6
bis(2-Chloroethyl)ether
Concen: 0.023 ng
RT: 7.143 min Scan# 430
Delta R.T. 0.000 min
Lab File: BN017908.D
Acq: 11 Dec 2021 15:58




Instrument :
BNA_N
ClientSampleId :
MW179D-20211206

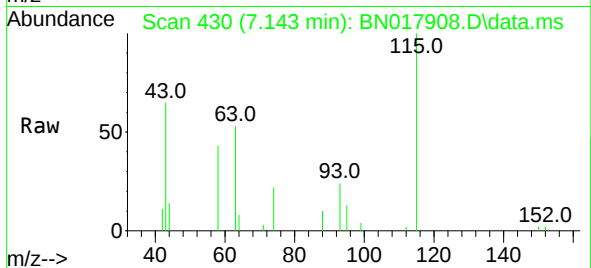


Tgt Ion: 93 Resp: 1420
Ion Ratio Lower Upper
93 100
63 227.3 62.0 93.0
95 53.5 26.2 39.4

Manual Integrations
APPROVED



Reviewed By :Christian Giraldo 12/15/2021
Supervised By :Yogesh Patel 12/16/2021

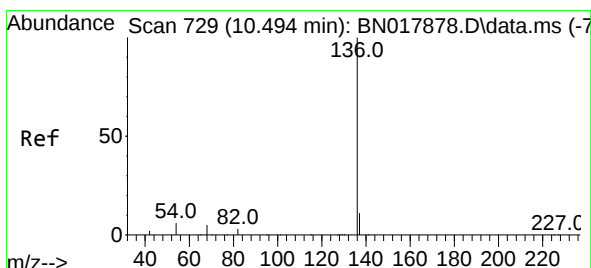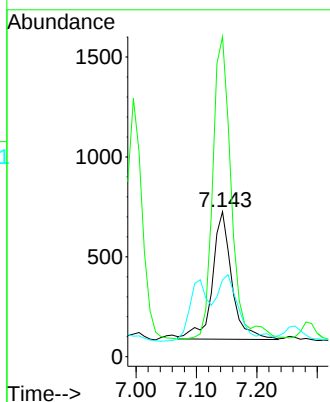


#7
Naphthalene-d8
Concen: 0.400 ng
RT: 10.494 min Scan# 729
Delta R.T. 0.000 min
Lab File: BN017908.D
Acq: 11 Dec 2021 15:58




Tgt Ion:136 Resp: 103116
Ion Ratio Lower Upper
136 100
137 11.0 8.8 13.2
54 6.4 5.1 7.7
68 5.5 4.4 6.6

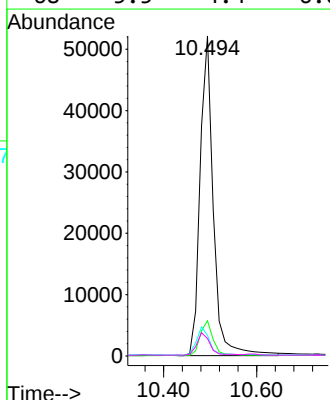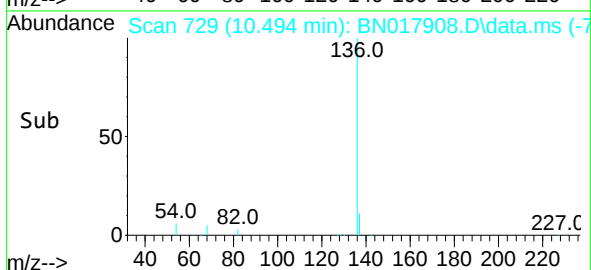



#8
Nitrobenzene-d5
Concen: 0.273 ng
RT: 8.859 min Scan# 600
Delta R.T. 0.000 min
Lab File: BN017908.D
Acq: 11 Dec 2021 15:58




Instrument :
BNA_N
ClientSampleId :
MW179D-20211206

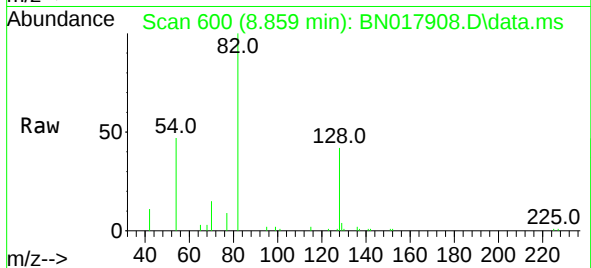

Tgt Ion: 82 Resp: 18369
Ion Ratio Lower Upper
82 100
128 41.7 32.2 48.4
54 46.7 37.6 56.4




Manual Integrations
APPROVED


Reviewed By :Christian Giraldo 12/15/2021
Supervised By :Yogesh Patel 12/16/2021

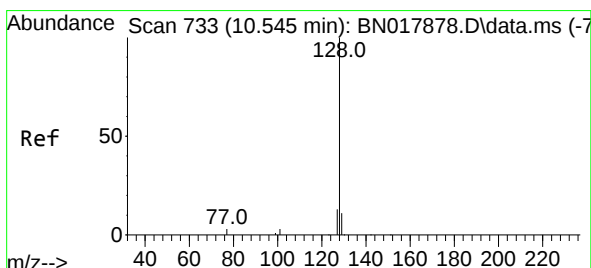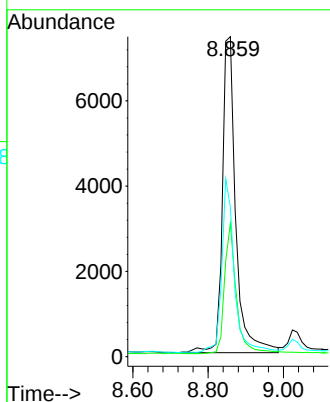

#9
Naphthalene
Concen: 0.035 ng
RT: 10.545 min Scan# 733
Delta R.T. -0.000 min
Lab File: BN017908.D
Acq: 11 Dec 2021 15:58

Tgt Ion:128 Resp: 9039
Ion Ratio Lower Upper
128 100
129 12.7 8.8 13.2
127 14.1 10.5 15.7

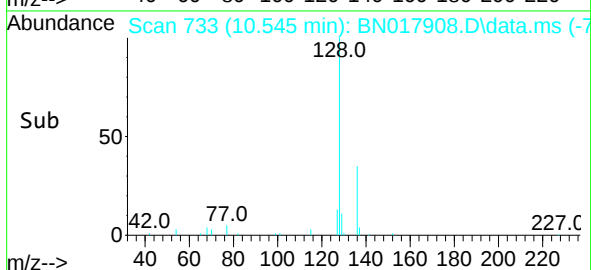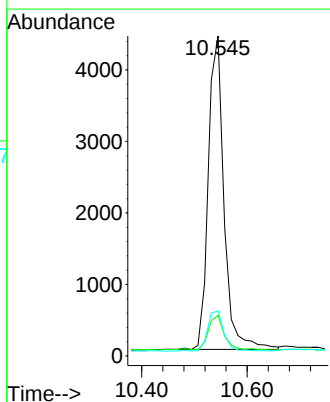

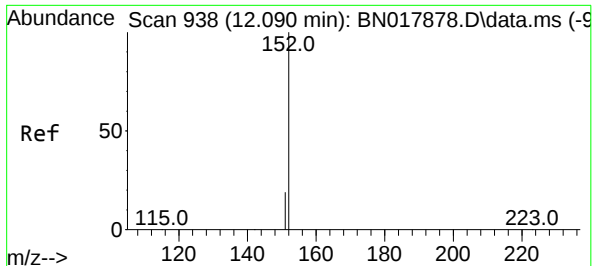





#11
2-Methylnaphthalene-d10
Concen: 0.257 ng
RT: 12.085 min Scan# 911
Delta R.T. -0.004 min
Lab File: BN017908.D
Acq: 11 Dec 2021 15:58

Instrument :
BNA_N
ClientSampleId :
MW179D-20211206

Tgt Ion:152 Resp: 4651
Ion Ratio Lower Upper
152 100
151 21.2 16.4 24.6




Manual Integrations
APPROVED


Reviewed By :Christian Giraldo 12/15/2021
Supervised By :Yogesh Patel 12/16/2021

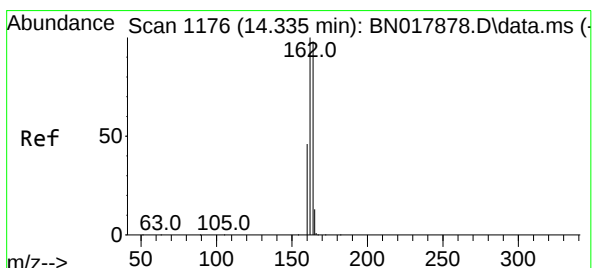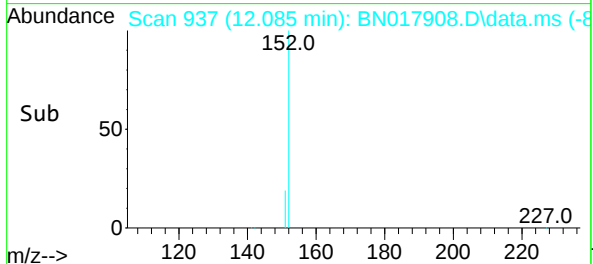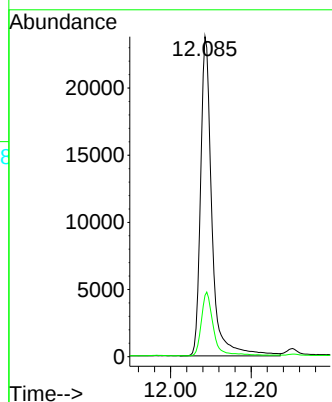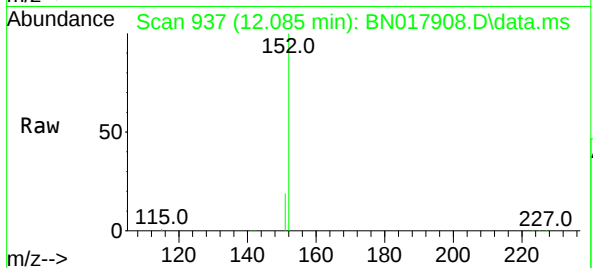

#13
Acenaphthene-d10
Concen: 0.400 ng
RT: 14.335 min Scan# 1176
Delta R.T. 0.000 min
Lab File: BN017908.D
Acq: 11 Dec 2021 15:58


Tgt Ion:164 Resp: 69754
Ion Ratio Lower Upper
164 100
162 101.6 82.1 123.1
160 46.4 38.2 57.2

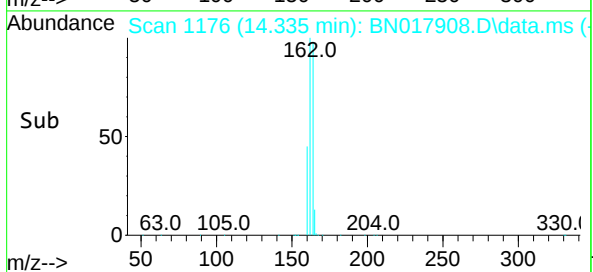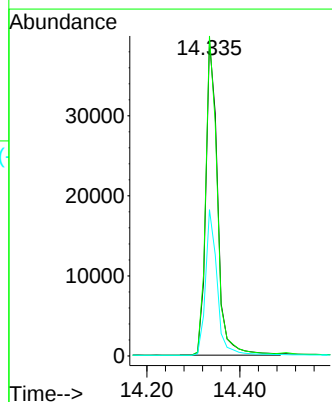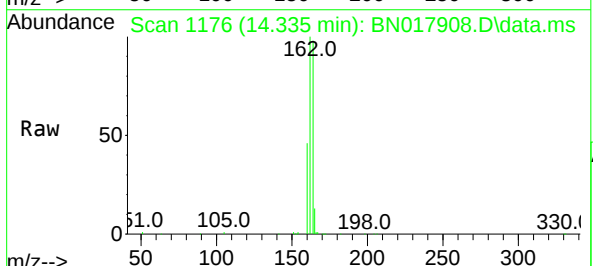



#14
2,4,6-Tribromophenol
Concen: 0.464 ng
RT: 15.844 min Scan# 1295
Delta R.T. 0.000 min
Lab File: BN017908.D
Acq: 11 Dec 2021 15:58




Instrument :
BNA_N
ClientSampleId :
MW179D-20211206

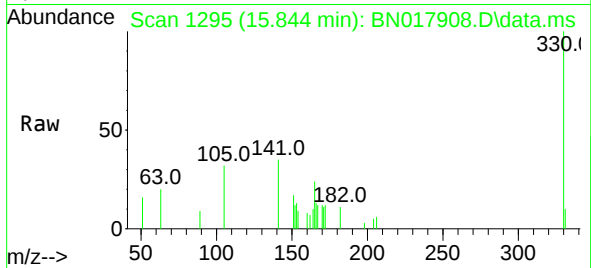


Tgt Ion:330 Resp: 4990
Ion Ratio Lower Upper
330 100
332 0.0 0.0 0.0
141 31.0 19.7 29.5

Manual Integrations
APPROVED



Reviewed By :Christian Giraldo 12/15/2021
Supervised By :Yogesh Patel 12/16/2021

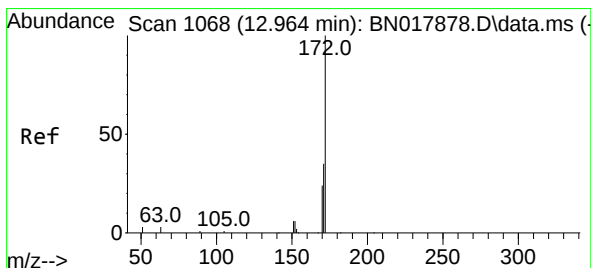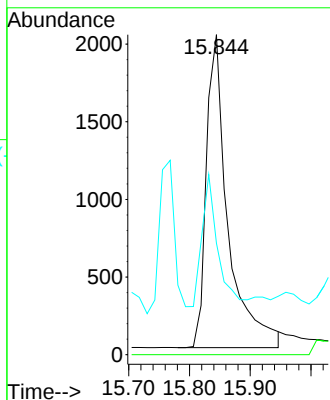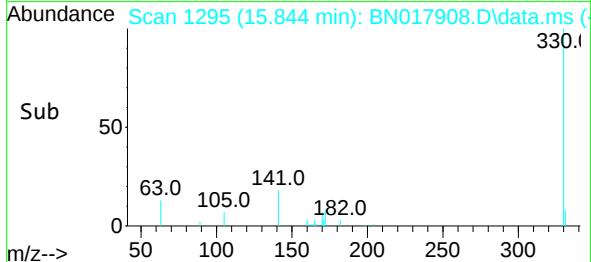


#15
2-Fluorobiphenyl
Concen: 0.298 ng
RT: 12.964 min Scan# 1068
Delta R.T. 0.000 min
Lab File: BN017908.D
Acq: 11 Dec 2021 15:58

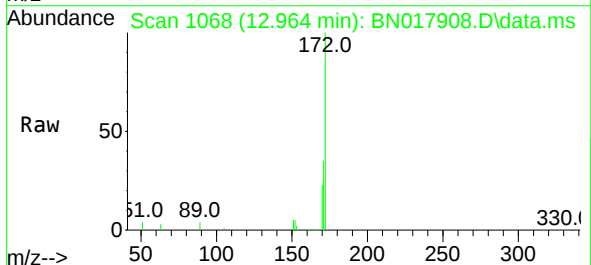


Tgt Ion:172 Resp: 73178
Ion Ratio Lower Upper
172 100
171 34.7 28.3 42.5
170 23.2 19.1 28.7

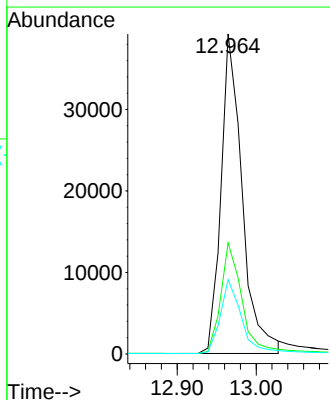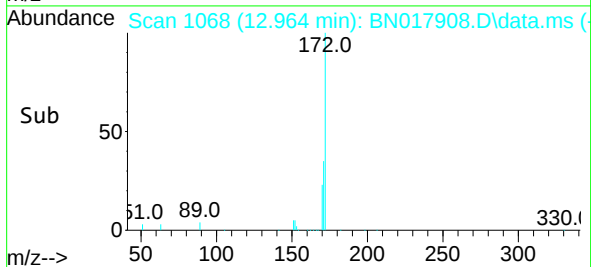

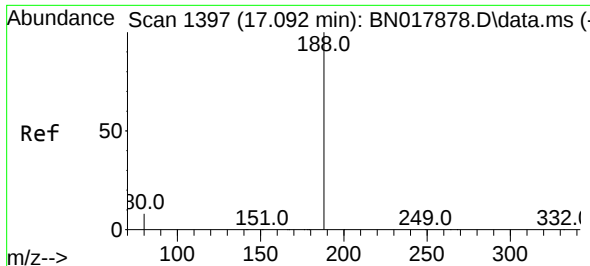

#19
Phenanthrene-d10
Concen: 0.400 ng
RT: 17.080 min Scan# 1396
Delta R.T. -0.012 min
Lab File: BN017908.D
Acq: 11 Dec 2021 15:58




Instrument :
BNA_N
ClientSampleId :
MW179D-20211206

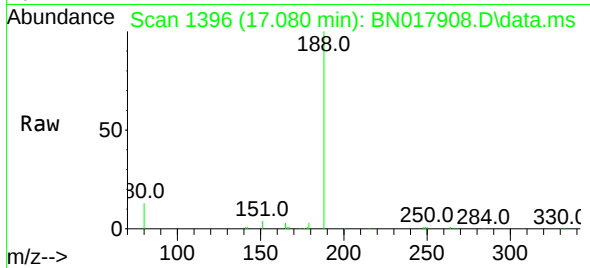

Tgt Ion:188 Resp: 136877
Ion Ratio Lower Upper
188 100
94 0.0 0.0 0.0
80 13.5 6.2 9.2




Manual Integrations
APPROVED


Reviewed By :Christian Giraldo 12/15/2021
Supervised By :Yogesh Patel 12/16/2021

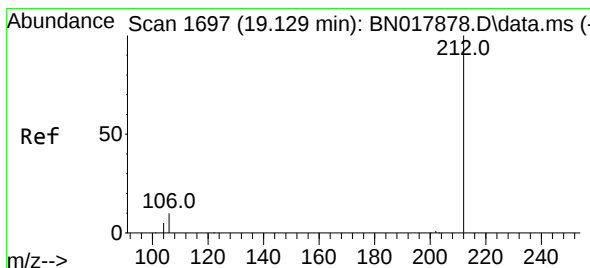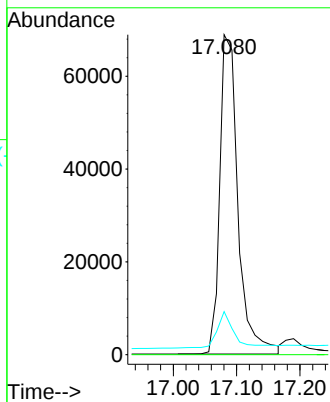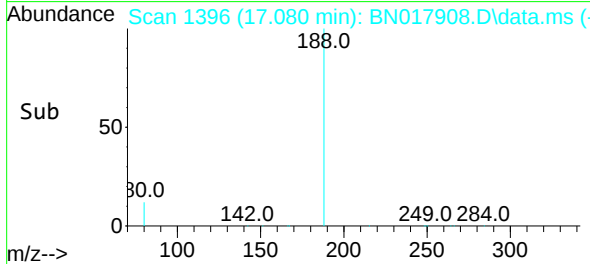

#27
Fluoranthene-d10
Concen: 0.310 ng
RT: 19.124 min Scan# 1696
Delta R.T. -0.005 min
Lab File: BN017908.D
Acq: 11 Dec 2021 15:58


Tgt Ion:212 Resp: 137579
Ion Ratio Lower Upper
212 100
106 9.8 8.3 12.5
104 5.3 4.6 6.8

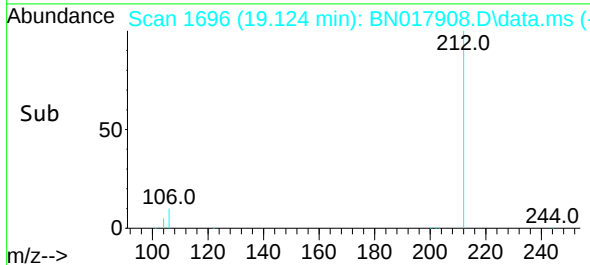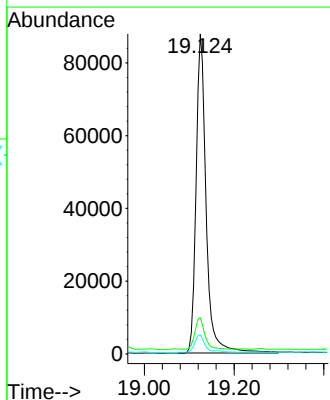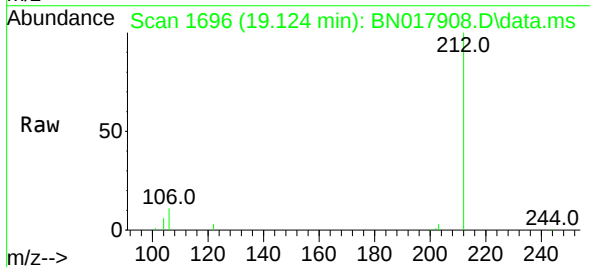

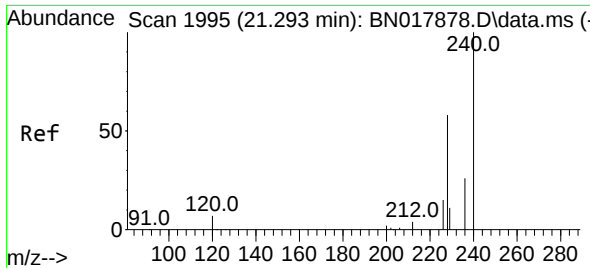

#29
Chrysene-d12
Concen: 0.400 ng
RT: 21.293 min Scan# 1995
Delta R.T. 0.000 min
Lab File: BN017908.D
Acq: 11 Dec 2021 15:58




Instrument :
BNA_N
ClientSampleId :
MW179D-20211206

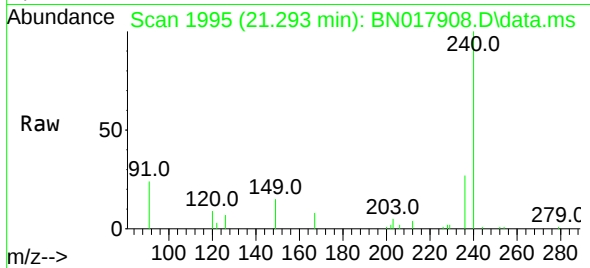


Tgt Ion:240 Resp: 97224
Ion Ratio Lower Upper
240 100
120 9.1 5.8 8.8
236 26.6 21.0 31.6

Manual Integrations
APPROVED



Reviewed By :Christian Giraldo 12/15/2021
Supervised By :Yogesh Patel 12/16/2021

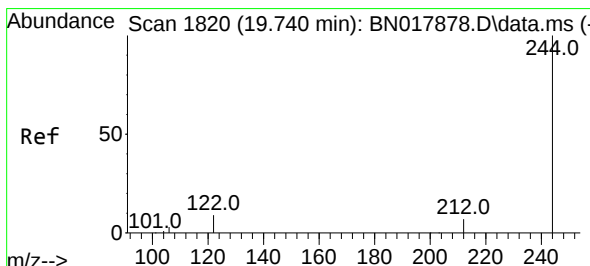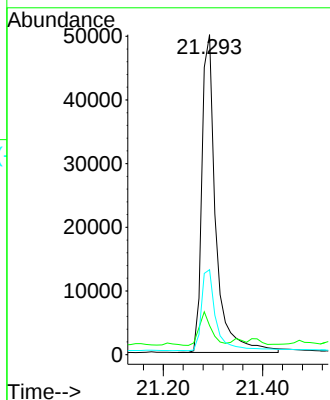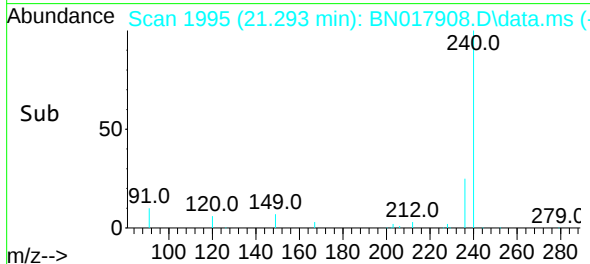


#31
Terphenyl-d14
Concen: 0.454 ng
RT: 19.730 min Scan# 1818
Delta R.T. -0.010 min
Lab File: BN017908.D
Acq: 11 Dec 2021 15:58

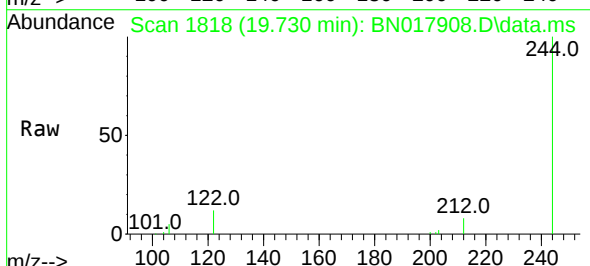


Tgt Ion:244 Resp: 108865
Ion Ratio Lower Upper
244 100
212 7.7 6.2 9.2
122 11.5 7.5 11.3

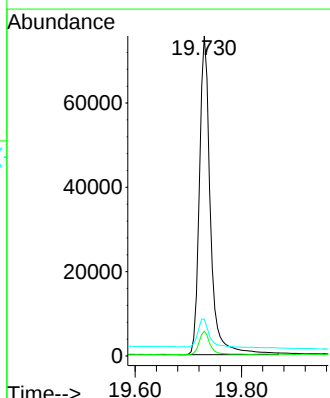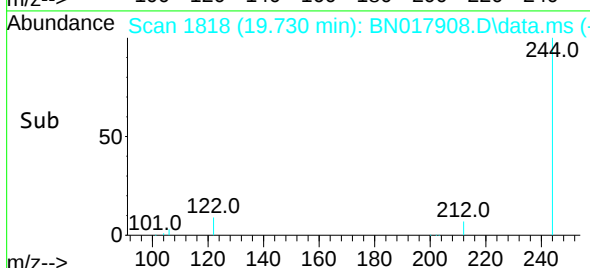

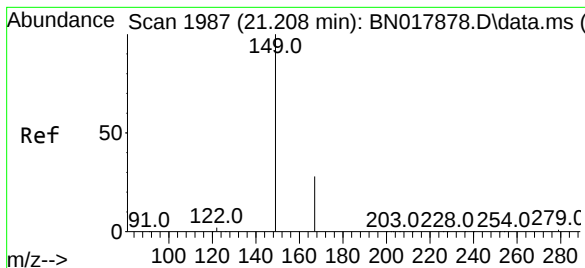

#34
Bis(2-ethylhexyl)phthalate
Concen: 10.018 ng
RT: 21.208 min Scan# 1987
Delta R.T. 0.000 min
Lab File: BN017908.D
Acq: 11 Dec 2021 15:58




Instrument :
BNA_N
ClientSampleId :
MW179D-20211206

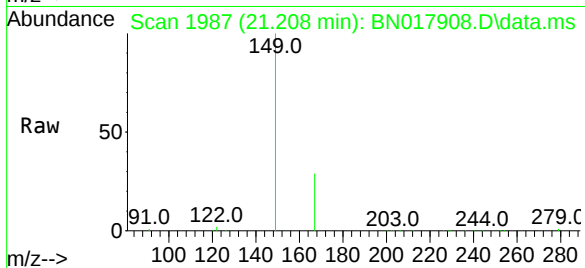

Tgt Ion:149 Resp: 104566
Ion Ratio Lower Upper
149 100
167 30.3 23.4 35.0
279 5.0 3.6 5.4




Manual Integrations
APPROVED


Reviewed By :Christian Giraldo 12/15/2021
Supervised By :Yogesh Patel 12/16/2021

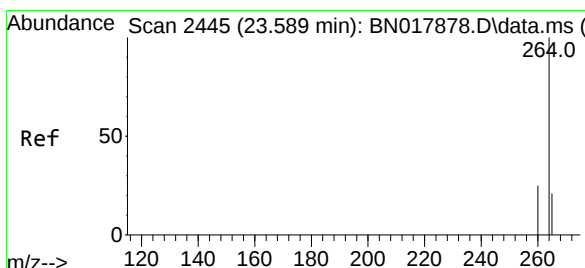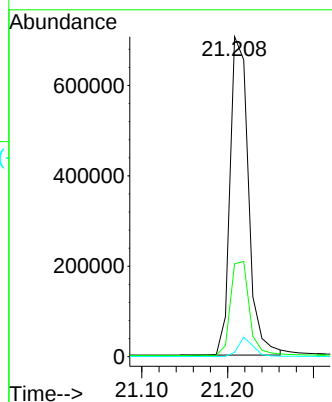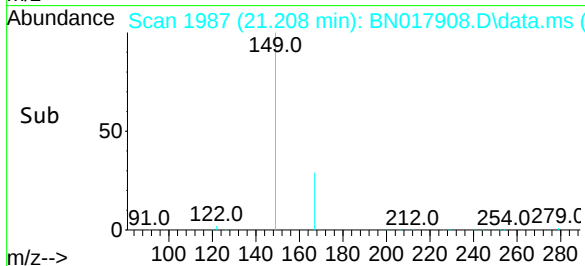

#35
Perylene-d12
Concen: 0.400 ng
RT: 23.589 min Scan# 2445
Delta R.T. 0.000 min
Lab File: BN017908.D
Acq: 11 Dec 2021 15:58


Tgt Ion:264 Resp: 77027
Ion Ratio Lower Upper
264 100
260 25.4 20.2 30.4
265 23.1 18.2 27.4

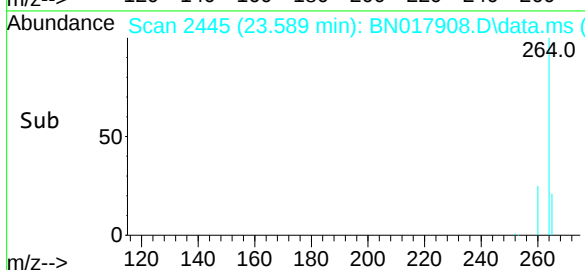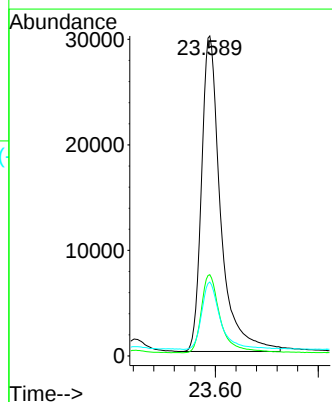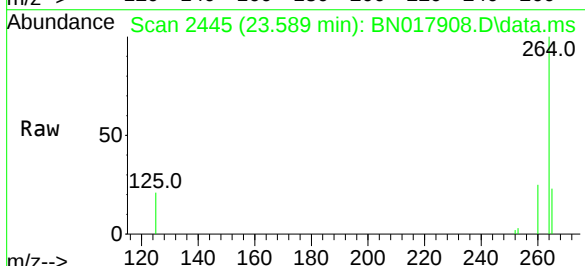

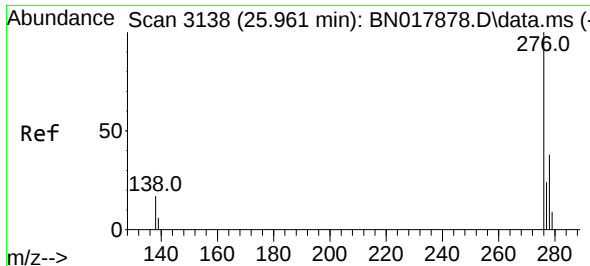

#36
Indeno(1,2,3-cd)pyrene
Concen: 0.097 ng
RT: 25.985 min Scan# 3145
Delta R.T. 0.024 min
Lab File: BN017908.D
Acq: 11 Dec 2021 15:58




Instrument :
BNA_N
ClientSampleId :
MW179D-20211206

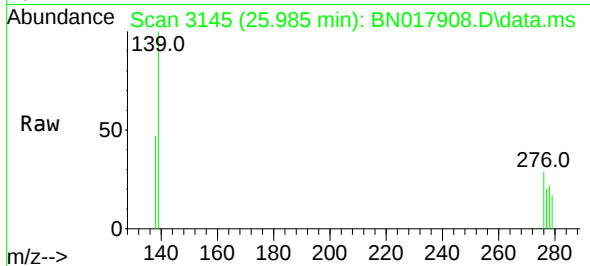


Tgt Ion:276 Resp: 125
Ion Ratio Lower Upper
276 100
138 0.0 15.2 22.8
277 6.0 19.8 29.6

Manual Integrations
APPROVED

Reviewed By :Christian Giraldo 12/15/2021
Supervised By :Yogesh Patel 12/16/2021

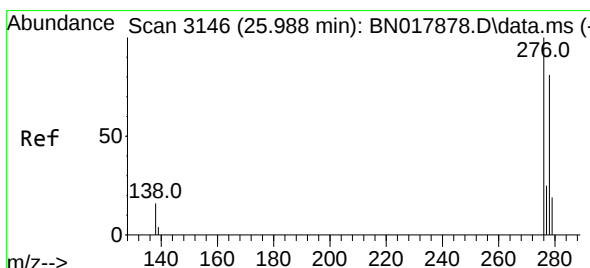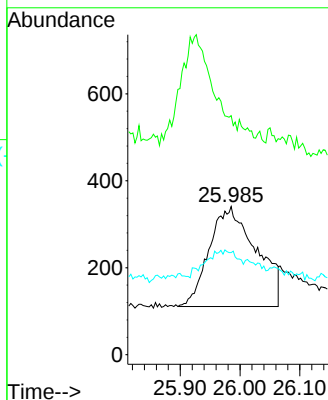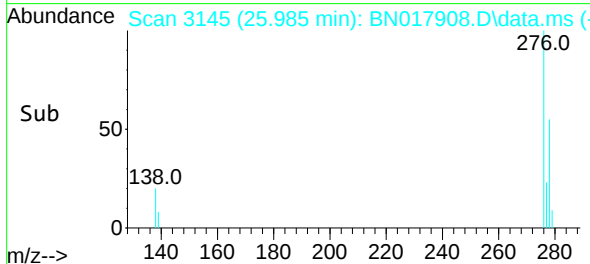

#40
Dibenzo(a,h)anthracene
Concen: 0.110 ng m
RT: 25.999 min Scan# 3149
Delta R.T. 0.011 min
Lab File: BN017908.D
Acq: 11 Dec 2021 15:58

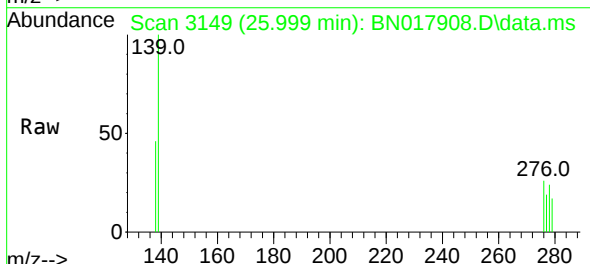

Tgt Ion:278 Resp: 975
Ion Ratio Lower Upper
278 100
139 412.7 12.0 18.0#
279 72.1 20.8 31.2#

