
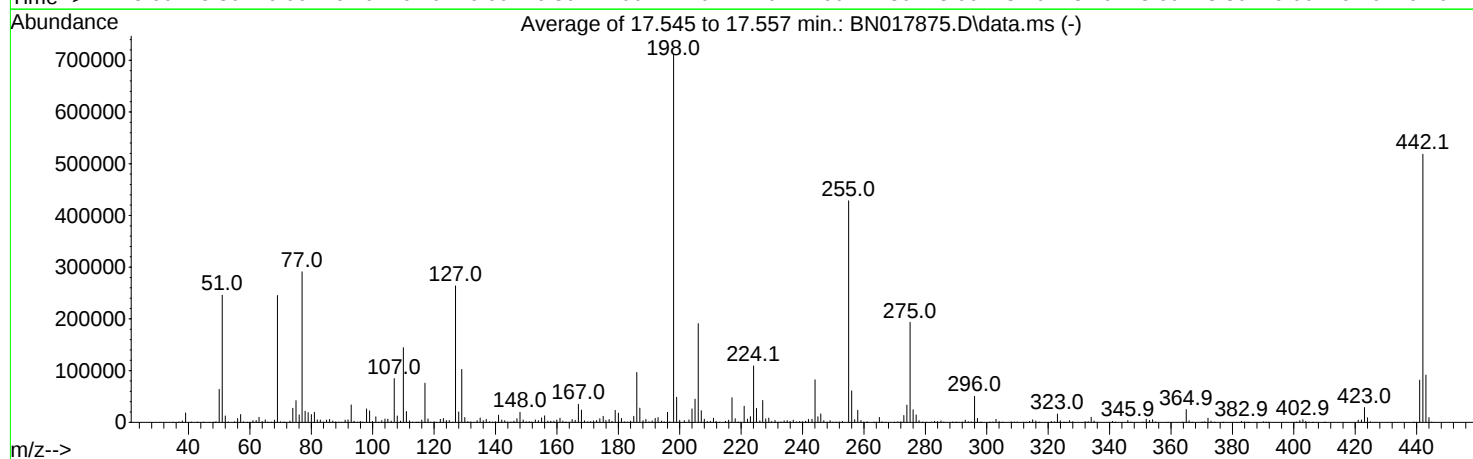


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121121\
 Data File : BN017875.D
 Acq On : 10 Dec 2021 17:39
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_N\METHODS\8270-SIM-BN121121.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Sat Dec 11 00:01:30 2021

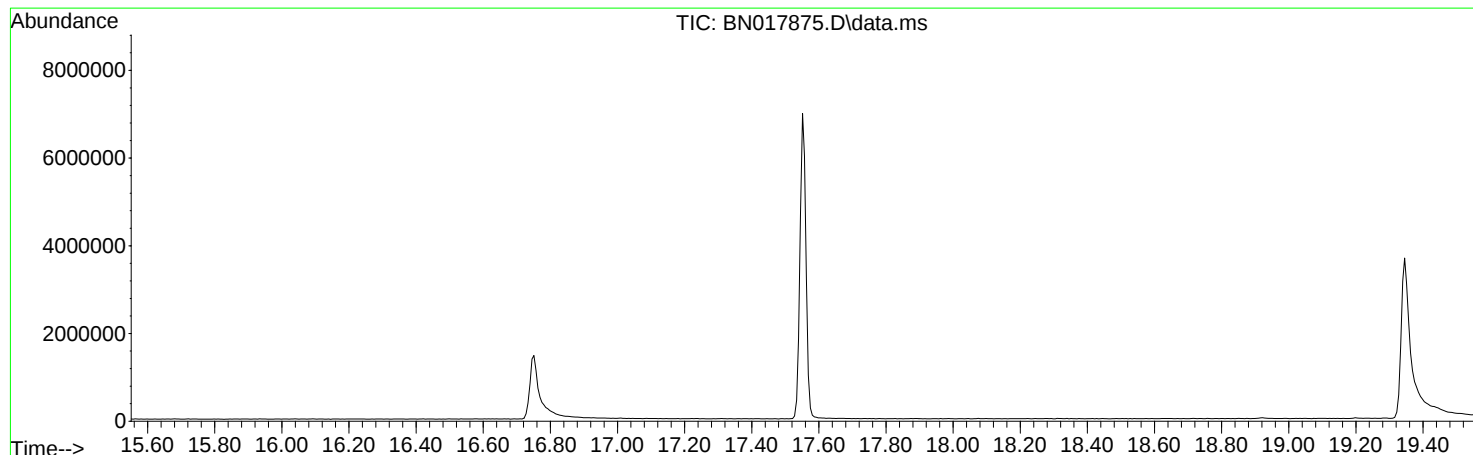




AutoFind: Scans 2475, 2476, 2477; Background Corrected with Scan 2468

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	34.6	245914	PASS
68	69	0.00	2	1.8	4330	PASS
69	198	0.00	100	34.5	245333	PASS
70	69	0.00	2	0.5	1273	PASS
127	198	10	80	37.1	263765	PASS
197	198	0.00	2	0.1	1007	PASS
198	198	100	100	100.0	711147	PASS
199	198	5	9	6.8	48587	PASS
275	198	10	60	27.2	193301	PASS
365	198	1	100	3.5	24795	PASS
441	198	0.01	100	11.5	81643	PASS
442	442	50	100	100.0	518571	PASS
443	442	15	24	17.7	91733	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121121\
Data File : BN017875.D
Acq On : 10 Dec 2021 17:39
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Dec 11 07:36:00 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Dec 11 07:33:12 2021
Response via : Initial Calibration

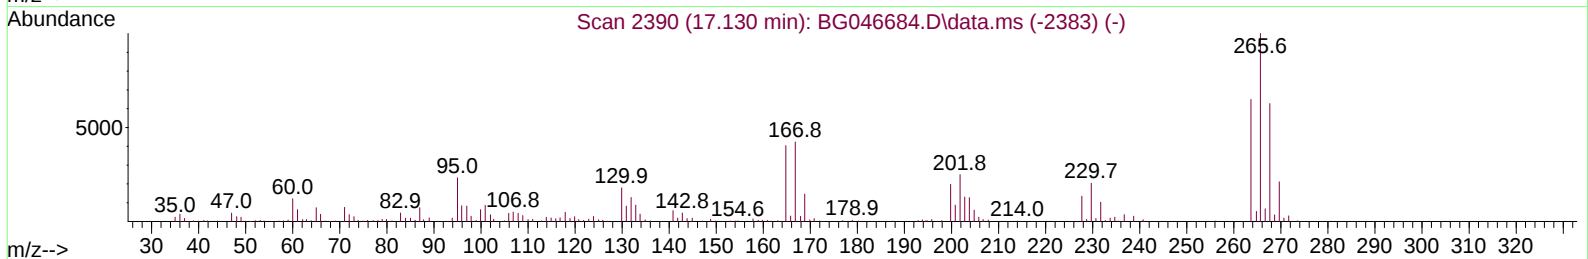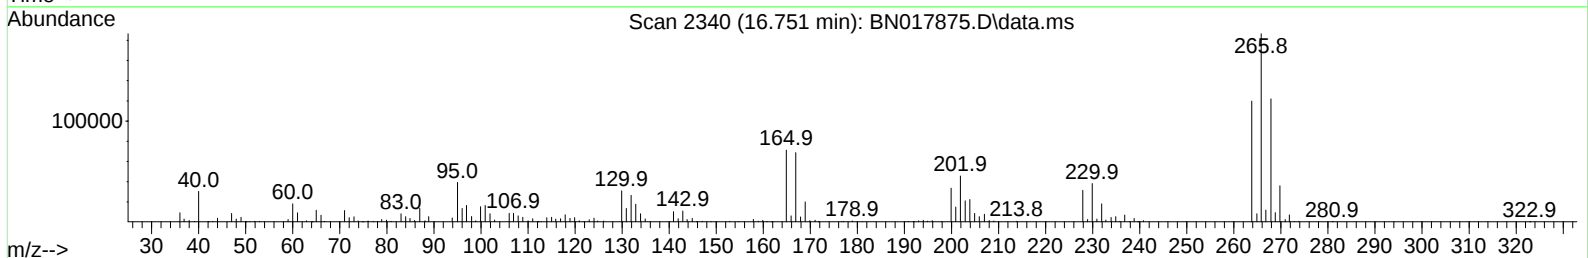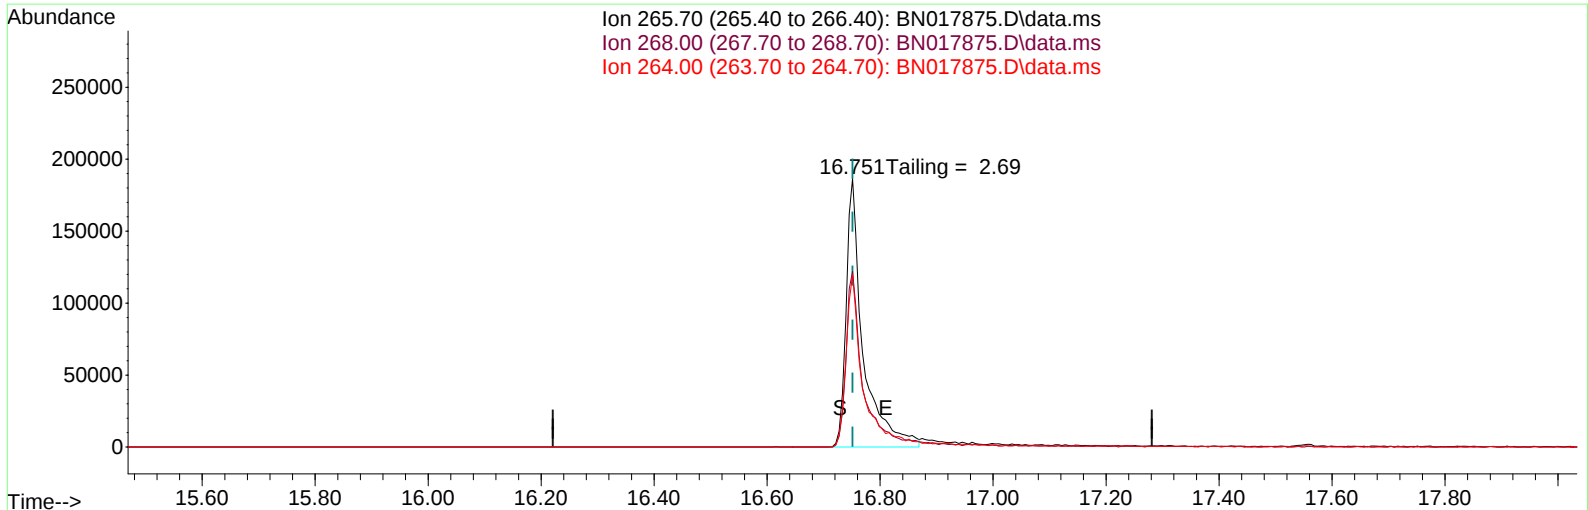

TIC: BN017875.D\data.ms

(70) Pentachlorophenol (C)

16.751min (-0.000) 10438.07 ng m




response 388934

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	65.39
264.00	61.60	64.27
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN121121\
 Data File : BN017875.D
 Acq On : 10 Dec 2021 17:39
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_N
 ClientSampleId :
 DFTPP

Quant Time: Dec 11 07:36:00 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Dec 11 07:33:12 2021
 Response via : Initial Calibration

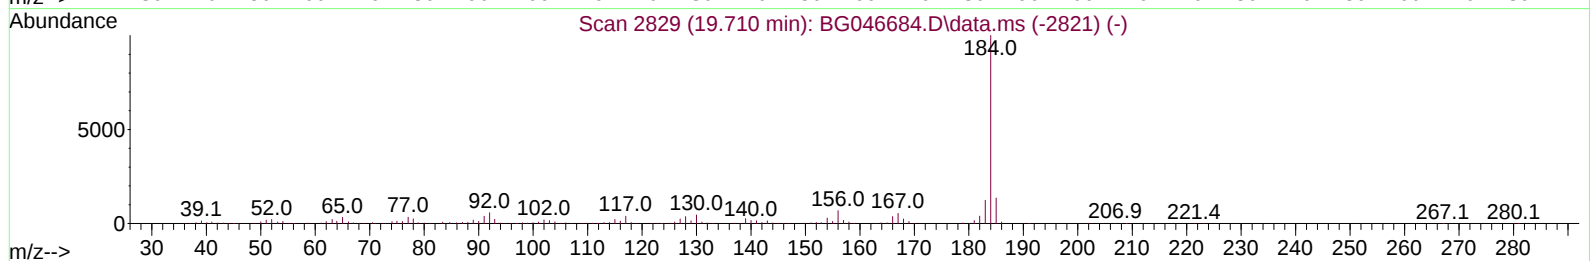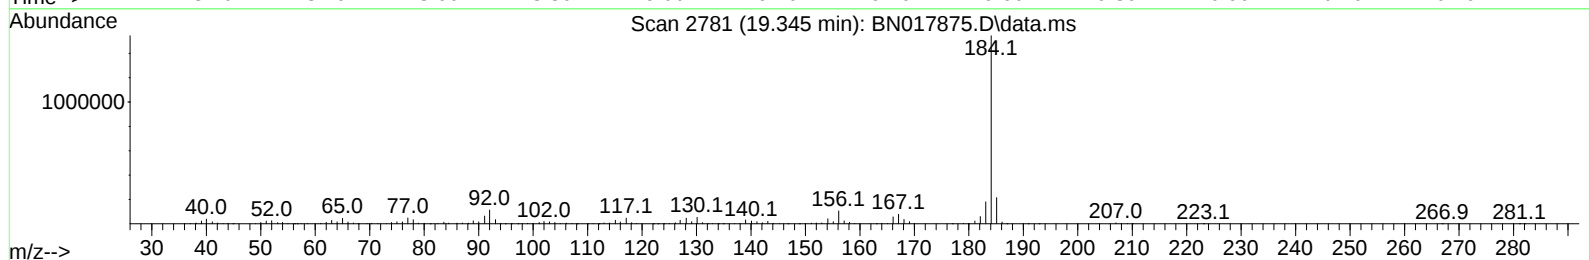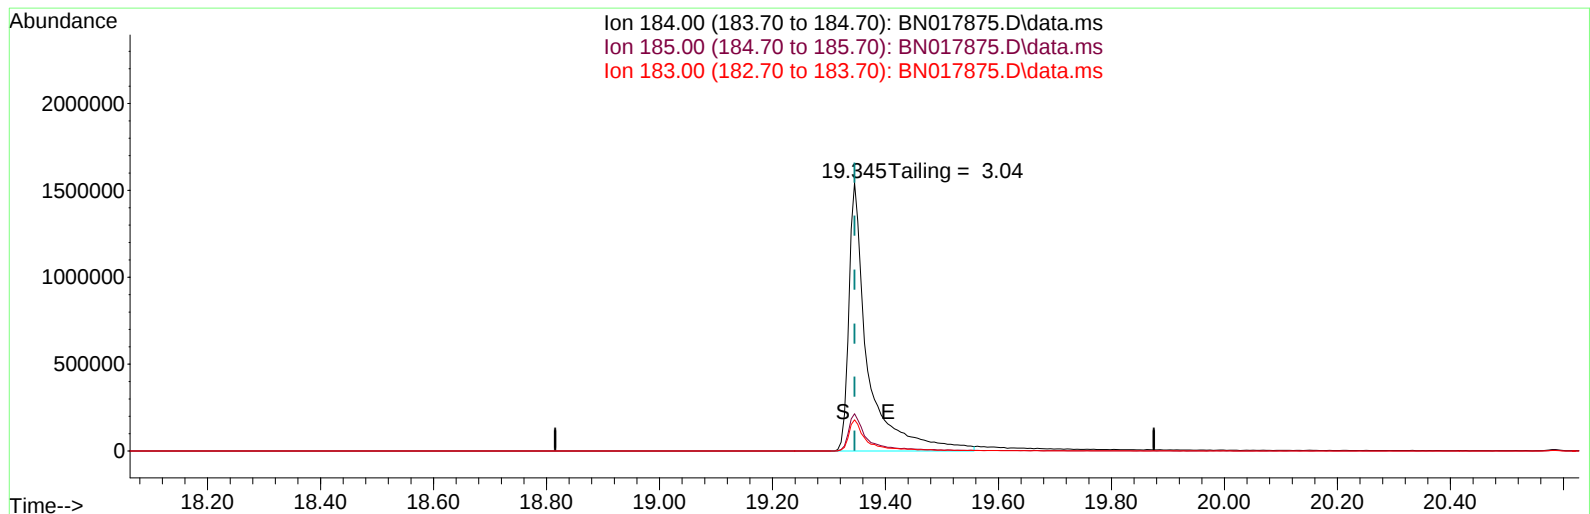

TIC: BN017875.D\data.ms

(77) Benzidine

19.345min (-0.000) 0.00 ng

response 3684339

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.93
183.00	13.20	11.64
0.00	0.00	0.00

Instrument :
BNA_N
ClientSampleId :
DFTPP

DDT Breakdown

Date	Instrument Name	DFTPP Data File
12/11/2021	BNA_N	<u>BN017875.D</u>
Compound Name	Response	Retention Time
DDT	2086237	20.586
DDD	92832	20.145
DDE	4974	19.639
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
97806	2184043	4.48

Instrument :
BNA_N
ClientSampleId :
DFTPP